

**Infrared Instrument
Weekly Calibration Verification Test Record**

Department: NISUP Morrsville Instrument Serial #: 160123

Test Date	Simulator Solution Lot #	Simulator Temperature			Sim. Serial#	Test Results			Breath Analysis Supervisor	Sim. Sol. Change *
		1	2	3		1	2	3		
10/27/17	17220	33.96	33.99	33.99	2017	.09	.09	.09	Bowman	
11/3/17	17220	33.97	34.00	33.98	2017	.09	.09	.09	Bowman	✓
11/11/17	17220	33.98	33.94	33.96	2017	.09	.09	.09	Duffy	
11/17/17	17220	33.96	34.01	33.94	2017	.09	.09	.09	DUFFY	
11/24/17	17220	33.94	33.95	33.96	2017	.09	.09	.09	Bowman	
12/1/17	17310	33.95	34.00	33.98	2017	.09	.09	.09	MACKO	✓
12/8/17	17310	33.97	33.97	34.01	2017	.09	.09	.09	Wright	
12/10/17	17310	33.96	33.99	33.97	2017	.09	.09	.09	MACKO	
12/22/17	17310	33.99	33.99	33.98	2017	.09	.09	.09	Bowman	
1/1/18	17310	33.97	34.00	34.00	2017	.09	.09	.09	Duffy	
1/8/18	17310	33.98	33.96	33.98	2017	.09	.09	.09	Wright	
1/12/18	17310	33.99	34.00	34.01	2017	.09	.09	.09	Bowman	✓

END
2017
BEGIN
2018

* - Please enter a ✓ to denote simulator solution change taking place

SUPERVISOR TEST




SUC MORRISVILLE
 UNIVERSITY POLICE
 DATAMASTER dmt: 100123

Date: 10/27/2017

Operator Name: RICHARD P BOWMAN
 Permit #: 44635
 Operator Agency/Dept: SUC MORRISVILLE PD
 Reference Standard #: 17220

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:15
INTERNAL STANDARD	VERIFIED	18:15
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	18:15
BLANK TEST	0.00	18:16
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	18:16
BLANK TEST	0.00	18:17
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	18:17
BLANK TEST	0.00	18:18

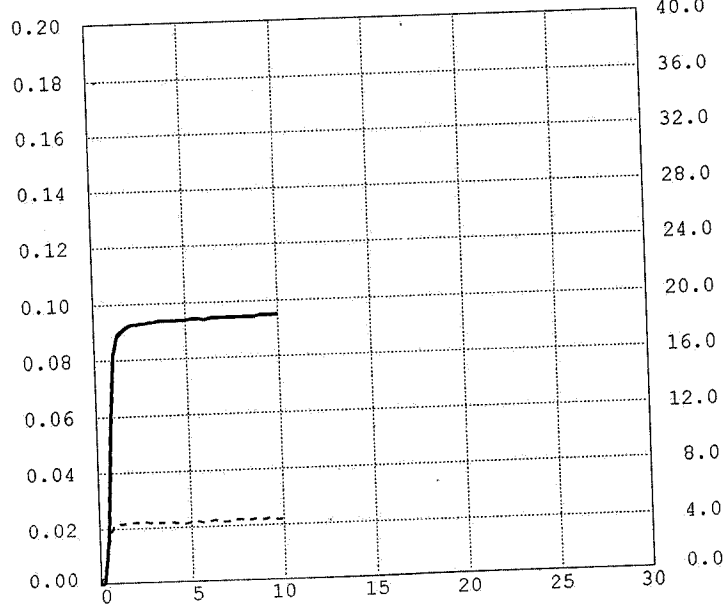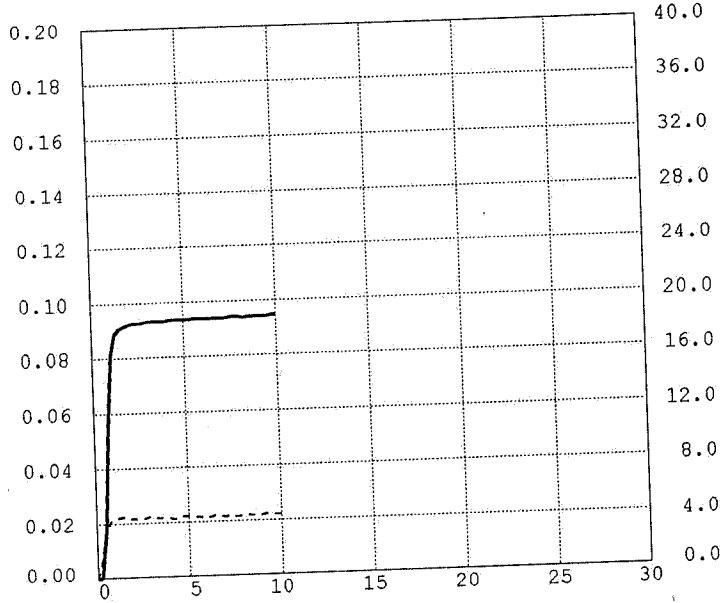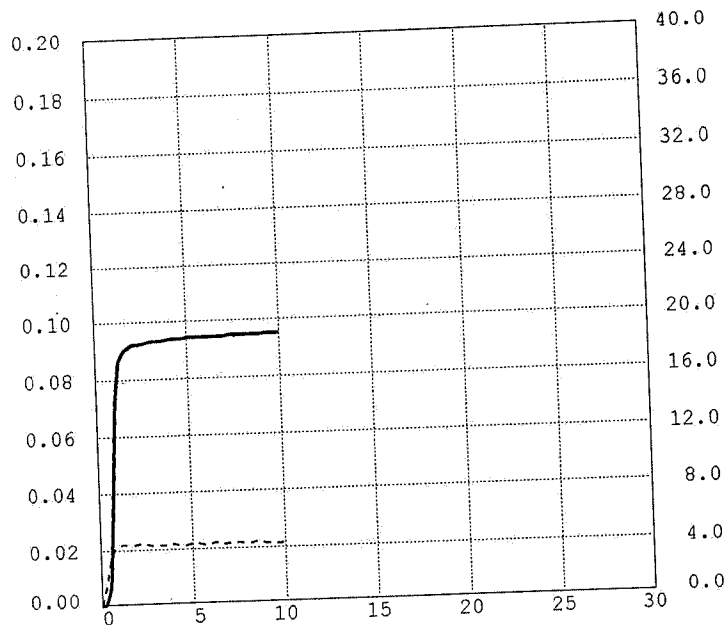

SOLUTION CHANGE




 SUC MORRISVILLE
 UNIVERSITY POLICE
 DATAMASTER dmt: 100123

Date: 11/03/2017

Operator Name: RICHARD P BOWMAN
 Permit #: 44635
 Operator Agency/Dept: SUC MORRISVILLE PD
 Reference Standard #: 17220

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:15
INTERNAL STANDARD	VERIFIED	05:15
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	05:16
BLANK TEST	0.00	05:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	05:17
BLANK TEST	0.00	05:17
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	05:18
BLANK TEST	0.00	05:18

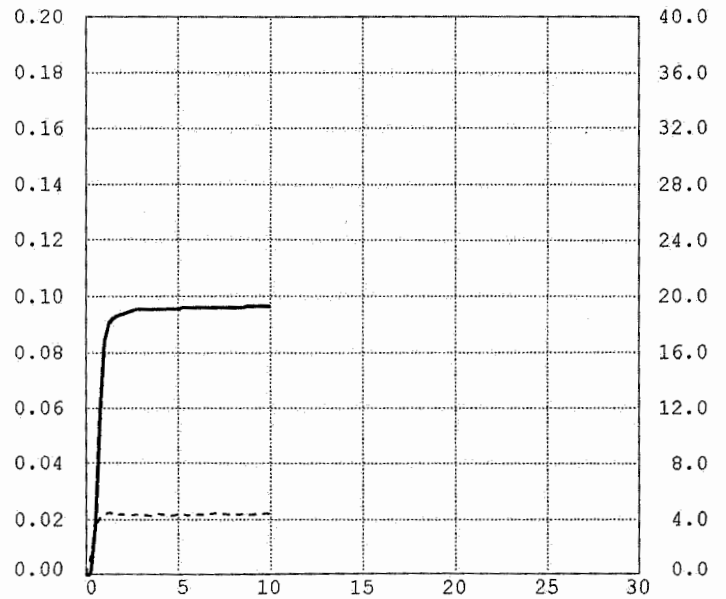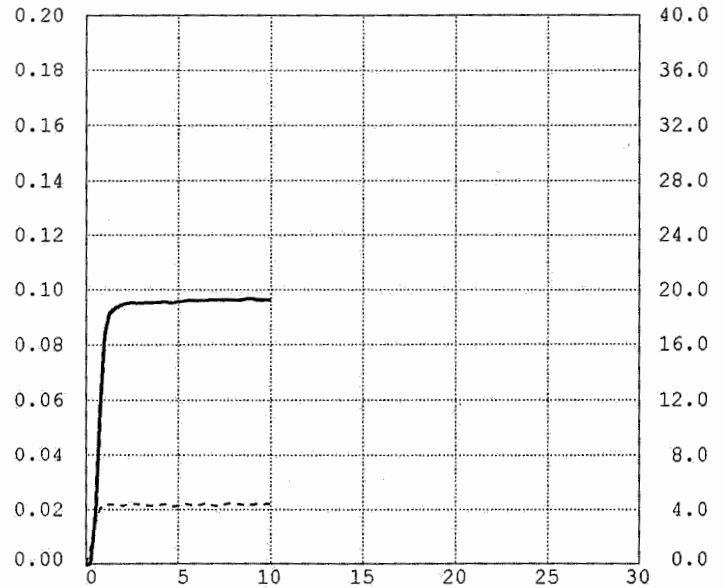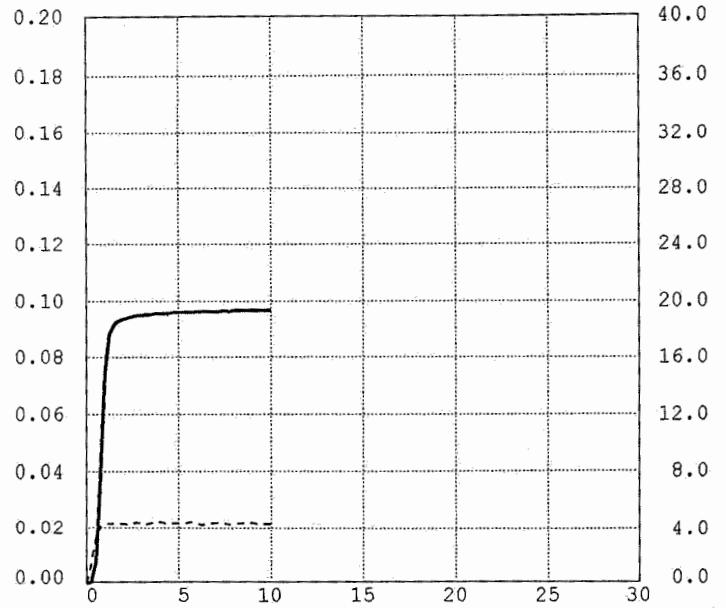

SUPERVISOR TEST




SUC MORRISVILLE
 UNIVERSITY POLICE
 DATAMASTER dmt: 100123

Date: 11/10/2017

Operator Name: CONOR J DUFFY
 Permit #: 39998
 Operator Agency/Dept: SUC MORRISVILLE PD
 Reference Standard #: 17220

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:31
INTERNAL STANDARD	VERIFIED	07:31
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	07:31
BLANK TEST	0.00	07:32
REFERENCE STANDARD TEMP	33.94c	
REFERENCE STANDARD	0.09	07:32
BLANK TEST	0.00	07:33
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	07:33
BLANK TEST	0.00	07:34

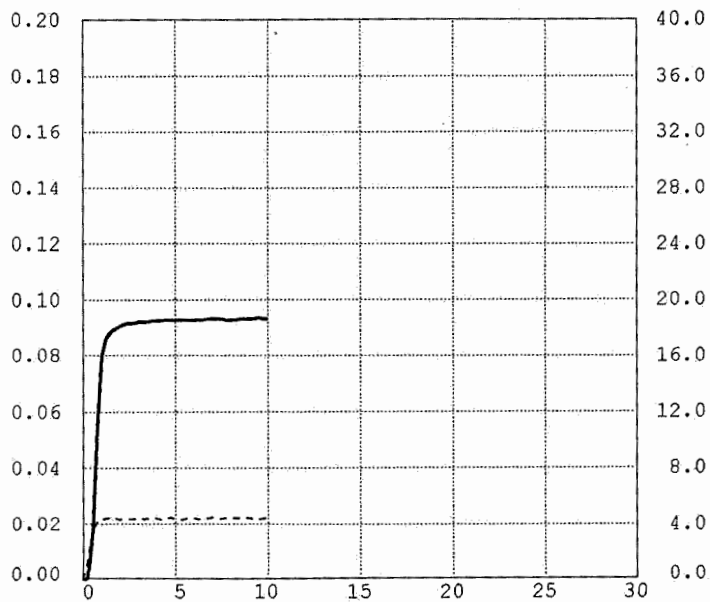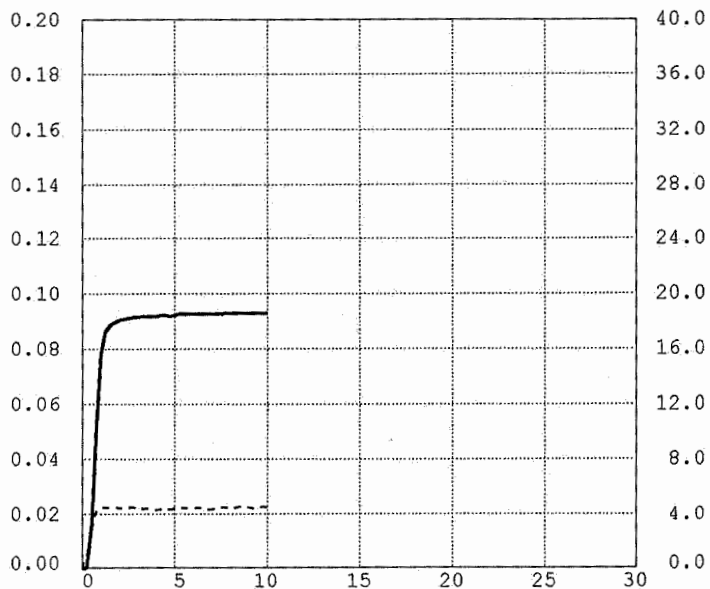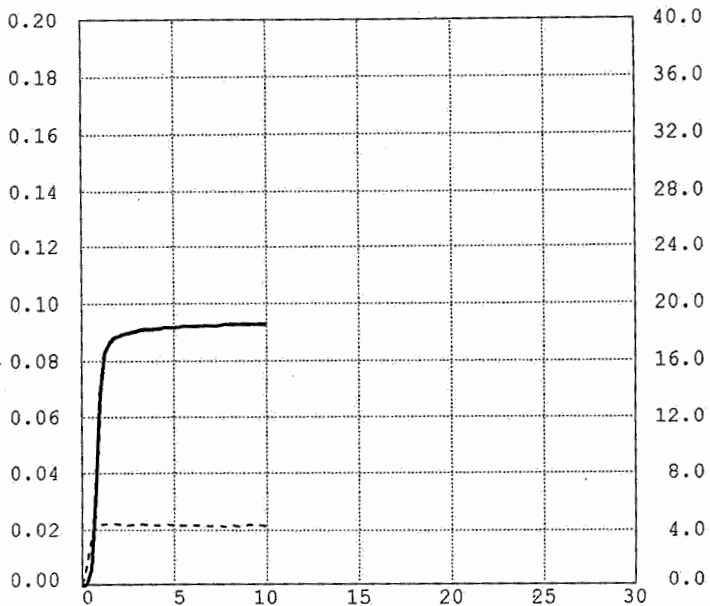

SUPERVISOR TEST




SUC MORRISVILLE
 UNIVERSITY POLICE
 DATAMASTER dmt: 100123

Date: 11/17/2017

Operator Name: CONOR J DUFFY
 Permit #: 39998
 Operator Agency/Dept: SUC MORRISVILLE PD
 Reference Standard #: 17220

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:30
INTERNAL STANDARD	VERIFIED	18:30
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	18:30
BLANK TEST	0.00	18:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:31
BLANK TEST	0.00	18:32
REFERENCE STANDARD TEMP	33.94c	
REFERENCE STANDARD	0.09	18:32
BLANK TEST	0.00	18:33

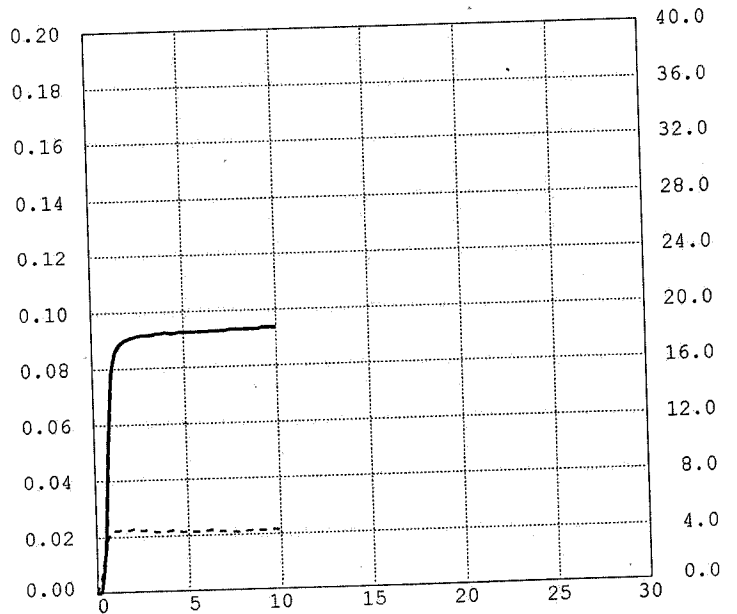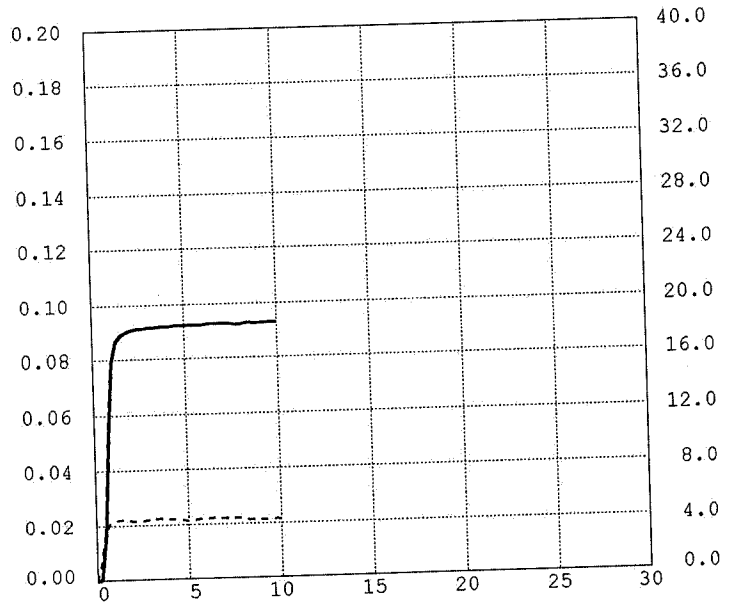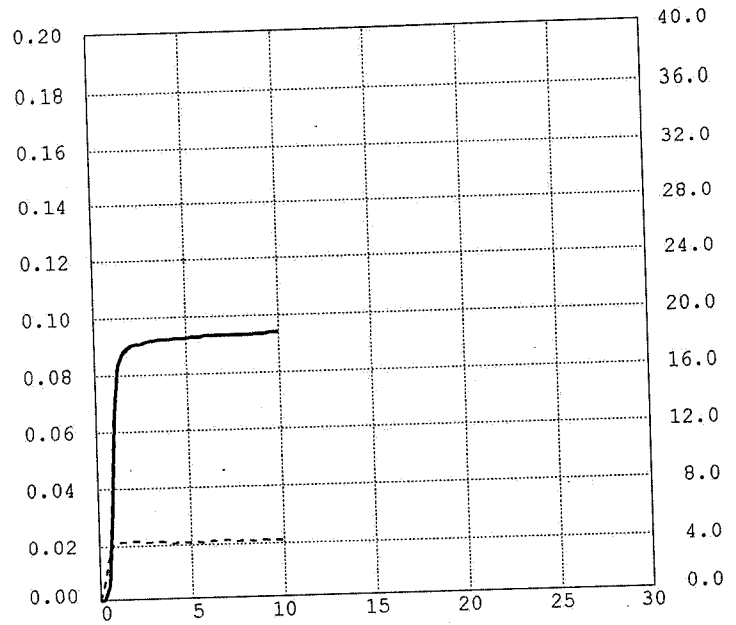

SUPERVISOR TEST




SUC MORRISVILLE
 UNIVERSITY POLICE
 DATAMASTER dmt: 100123

Date: 11/24/2017

Operator Name: RICHARD P BOWMAN
 Permit #: 44635
 Operator Agency/Dept: SUC MORRISVILLE PD
 Reference Standard #: 17220

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:47
INTERNAL STANDARD	VERIFIED	11:48
REFERENCE STANDARD TEMP	33.94c	
REFERENCE STANDARD	0.09	11:48
BLANK TEST	0.00	11:49
REFERENCE STANDARD TEMP	33.95c	
REFERENCE STANDARD	0.09	11:49
BLANK TEST	0.00	11:50
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	11:50
BLANK TEST	0.00	11:51

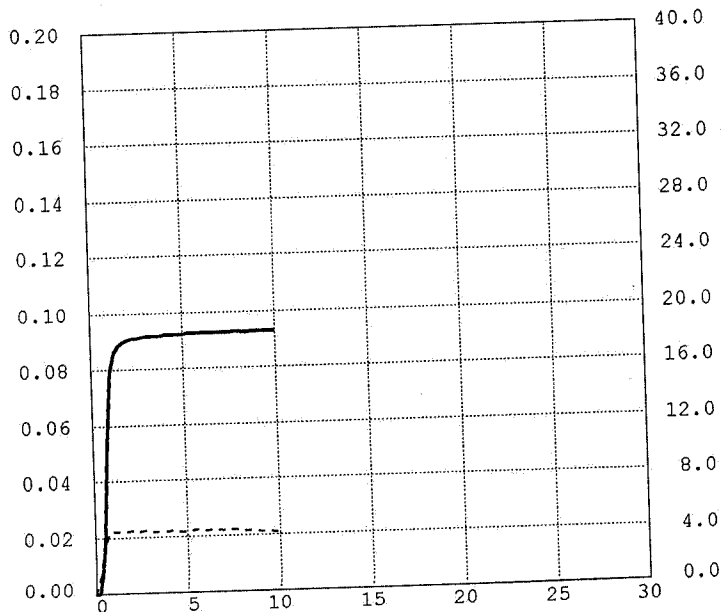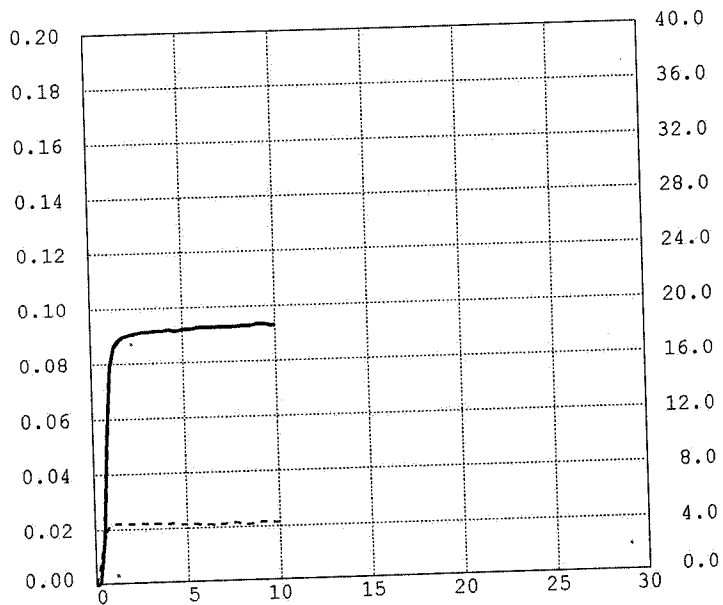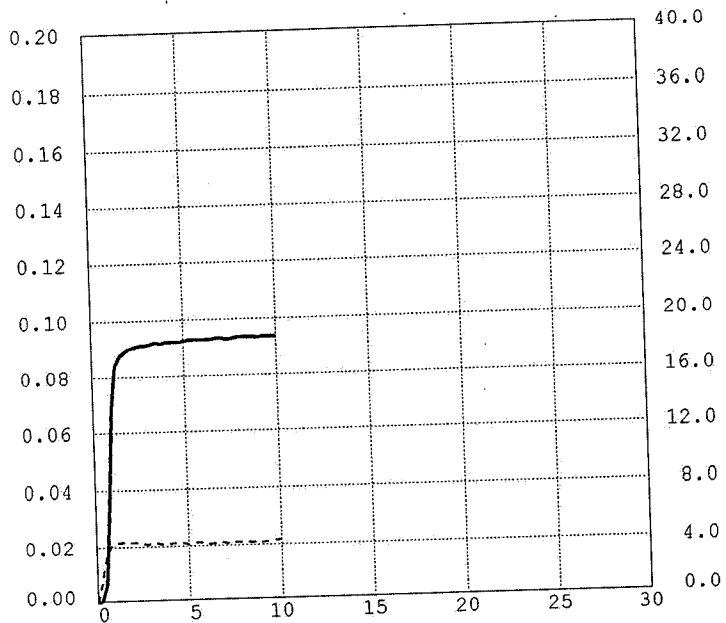

SOLUTION CHANGE




 SUC MORRISVILLE
 UNIVERSITY POLICE
 DATAMASTER dmt: 100123

Date: 12/01/2017

Operator Name: JONATHAN S MACKO
 Permit #: 45982
 Operator Agency/Dept: SUC MORRISVILLE PD
 Reference Standard #: 17310

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:58
INTERNAL STANDARD	VERIFIED	21:59
REFERENCE STANDARD TEMP	33.93c	
REFERENCE STANDARD	0.09	21:59
BLANK TEST	0.00	22:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:00
BLANK TEST	0.00	22:01
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	22:01
BLANK TEST	0.00	22:02

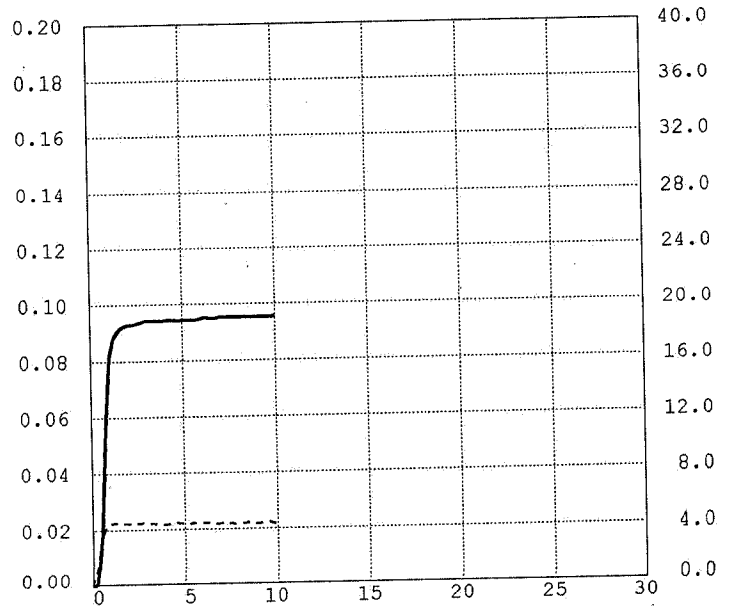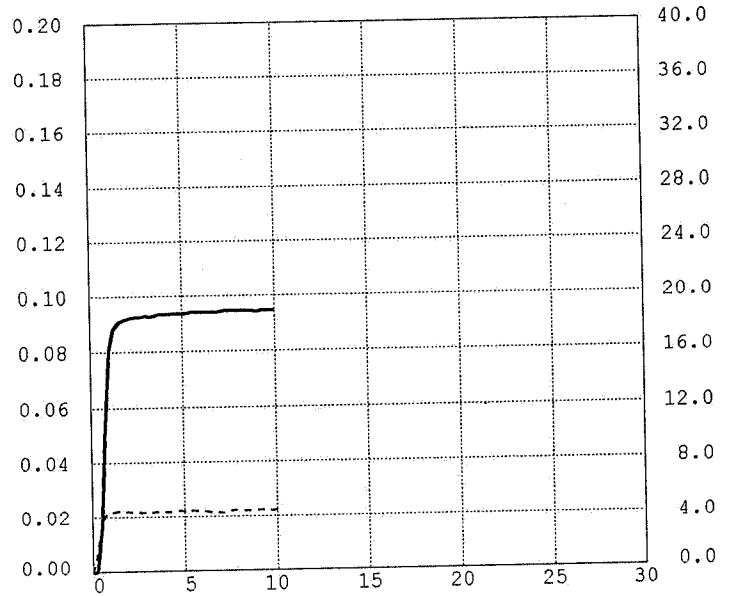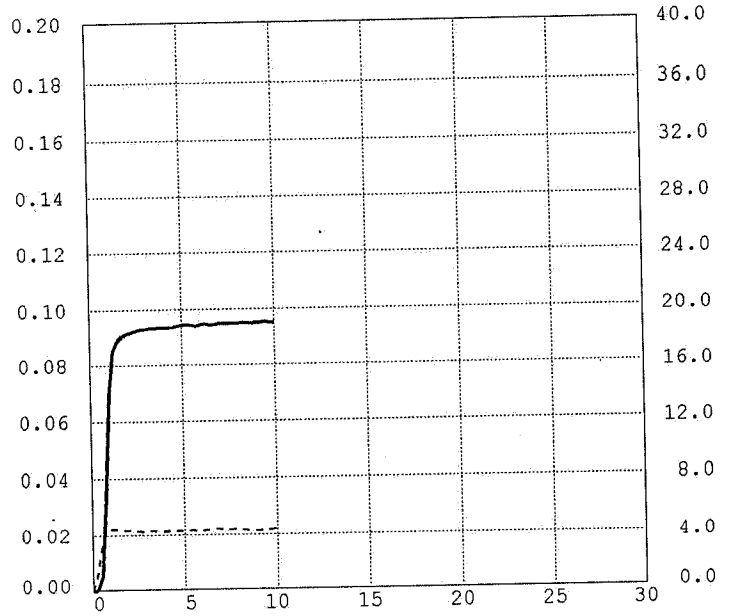

SUPERVISOR TEST




 SUC MORRISVILLE
 UNIVERSITY POLICE
 DATAMASTER dmt: 100123

Date: 12/08/2017

Operator Name: NICOLE M WRIGHT
 Permit #: 41034
 Operator Agency/Dept: SUC MORRISVILLE PD
 Reference Standard #: 17310

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:41
INTERNAL STANDARD	VERIFIED	22:41
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	22:42
BLANK TEST	0.00	22:42
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	22:43
BLANK TEST	0.00	22:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:44
BLANK TEST	0.00	22:44

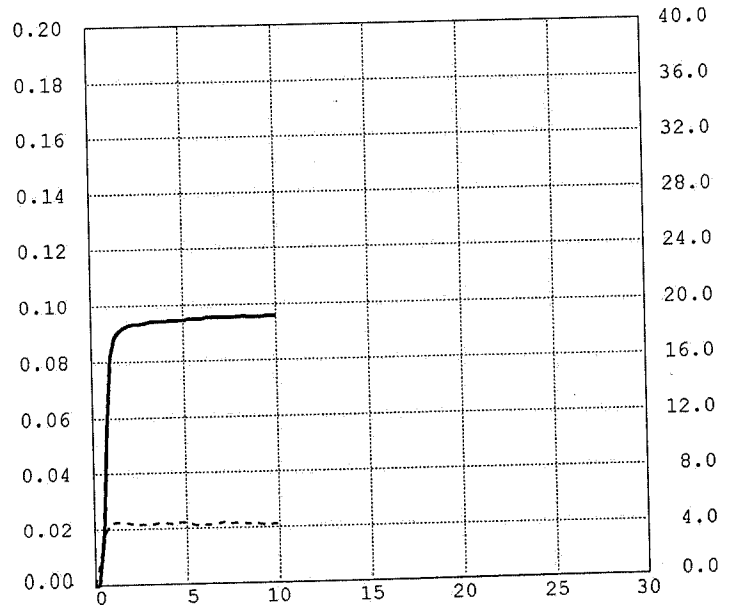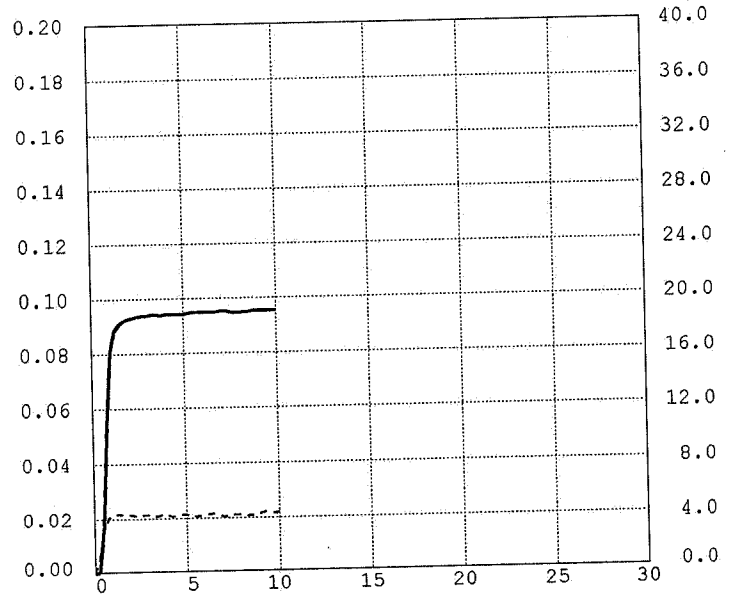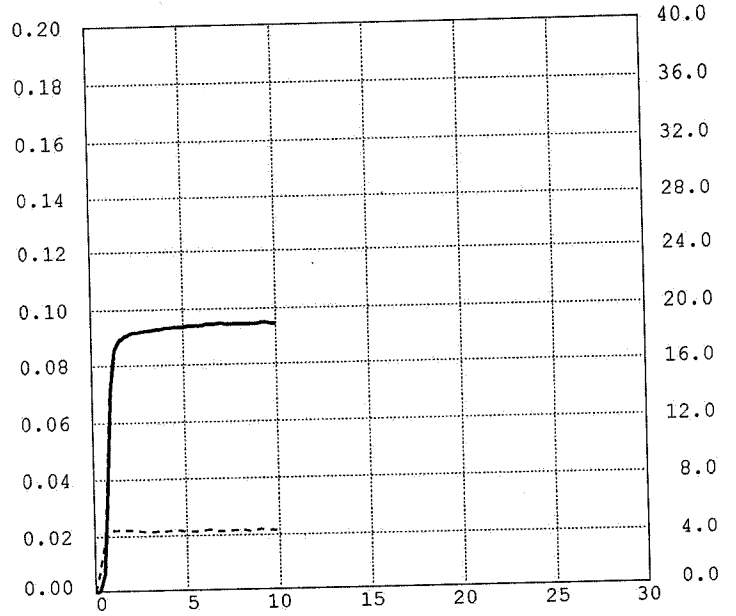

SUPERVISOR TEST




SUC MORRISVILLE
 UNIVERSITY POLICE
 DATAMASTER dmt: 100123

Date: 12/16/2017

Operator Name: JONATHAN S MACKO
 Permit #: 45982
 Operator Agency/Dept: SUC MORRISVILLE PD
 Reference Standard #: 17310

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:28
INTERNAL STANDARD	VERIFIED	11:28
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	11:28
BLANK TEST	0.00	11:29
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:29
BLANK TEST	0.00	11:30
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	11:30
BLANK TEST	0.00	11:31

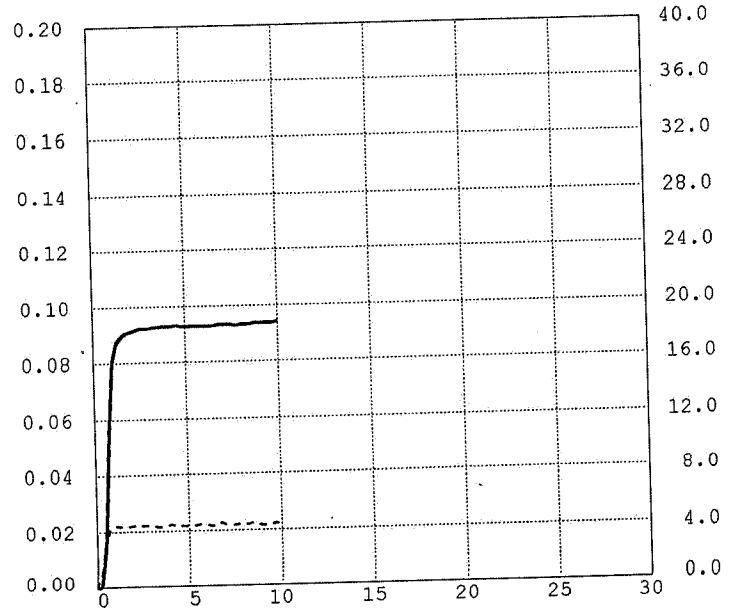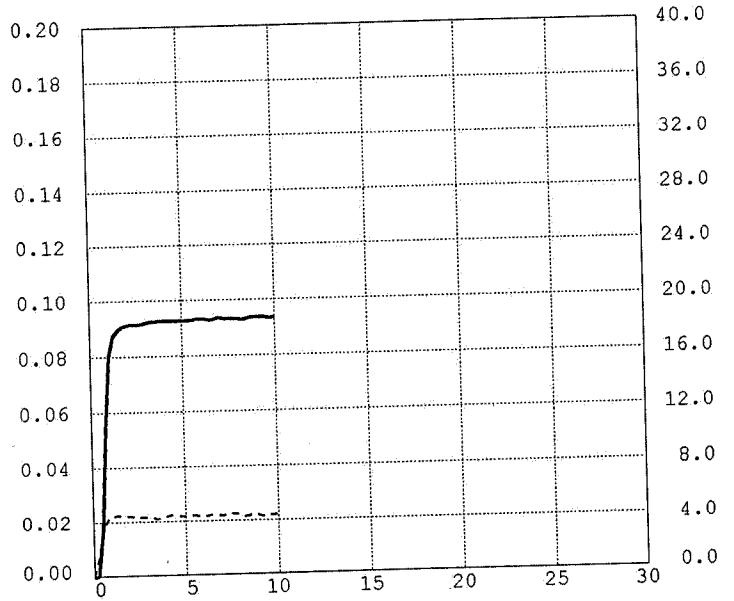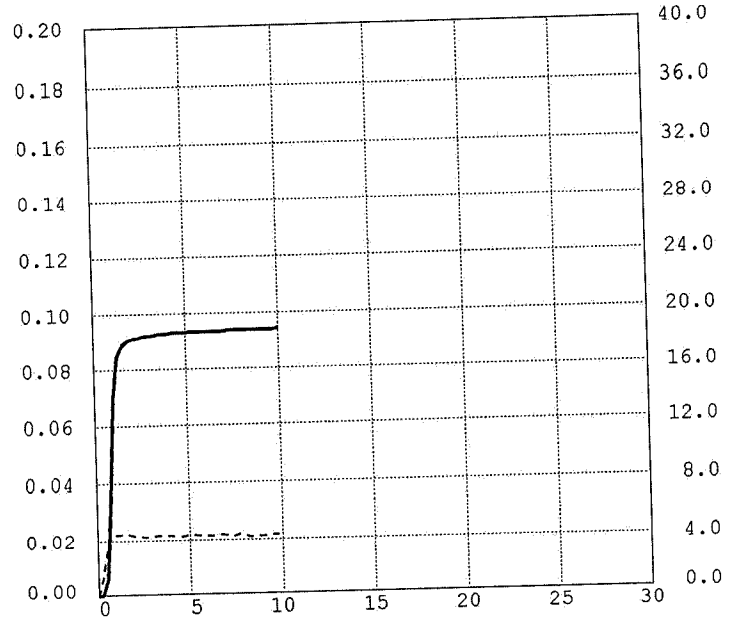

SUPERVISOR TEST




 SUC MORRISVILLE
 UNIVERSITY POLICE
 DATAMASTER dmt: 100123

Date: 12/22/2017

Operator Name: RICHARD P BOWMAN
 Permit #: 44635
 Operator Agency/Dept: SUC MORRISVILLE PD
 Reference Standard #: 17310

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:09
INTERNAL STANDARD	VERIFIED	13:09
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	13:10
BLANK TEST	0.00	13:11
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	13:11
BLANK TEST	0.00	13:12
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	13:12
BLANK TEST	0.00	13:13

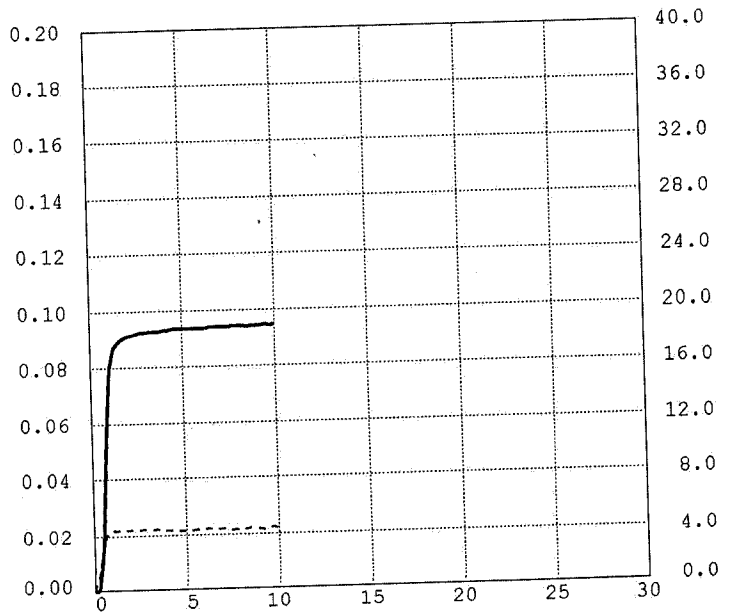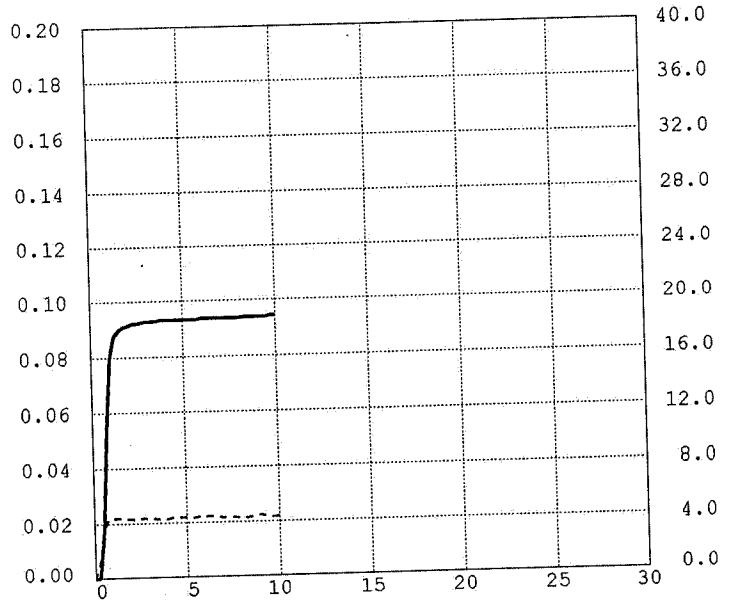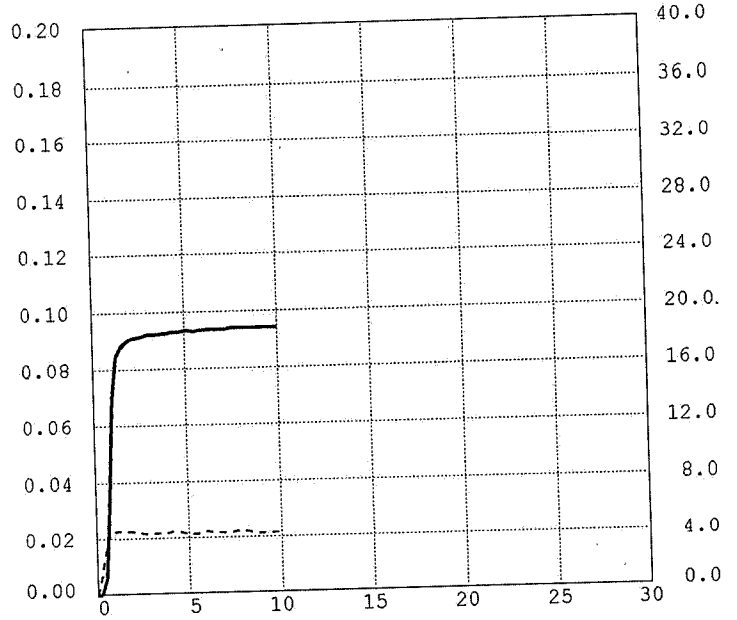

SUPERVISOR TEST




SUC MORRISVILLE
 UNIVERSITY POLICE
 DATAMASTER dmt: 100123

Date: 01/01/2018

Operator Name: CONOR J DUFFY
 Permit #: 39998
 Operator Agency/Dept: SUC MORRISVILLE PD
 Reference Standard #: 17310

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:16
INTERNAL STANDARD	VERIFIED	15:16
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	15:16
BLANK TEST	0.00	15:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:17
BLANK TEST	0.00	15:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:19
BLANK TEST	0.00	15:19

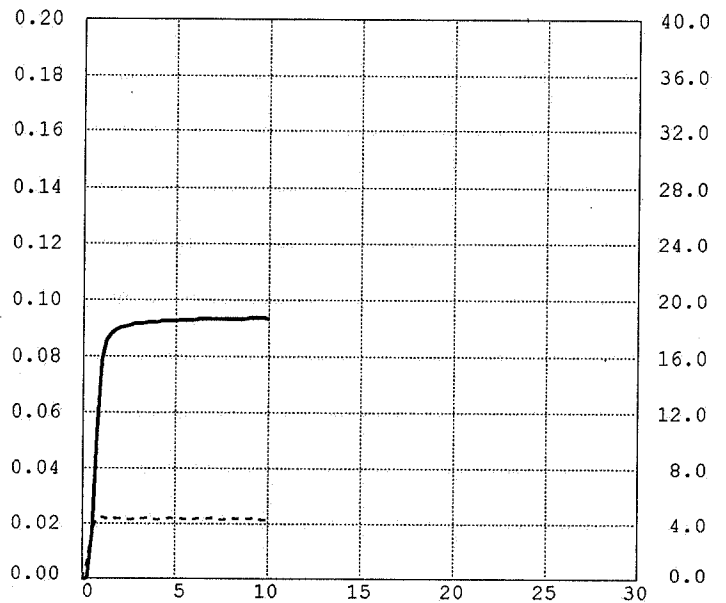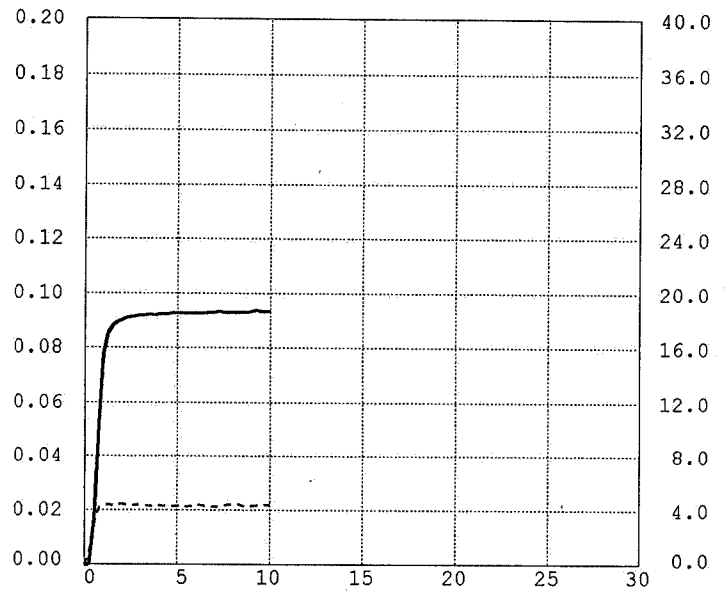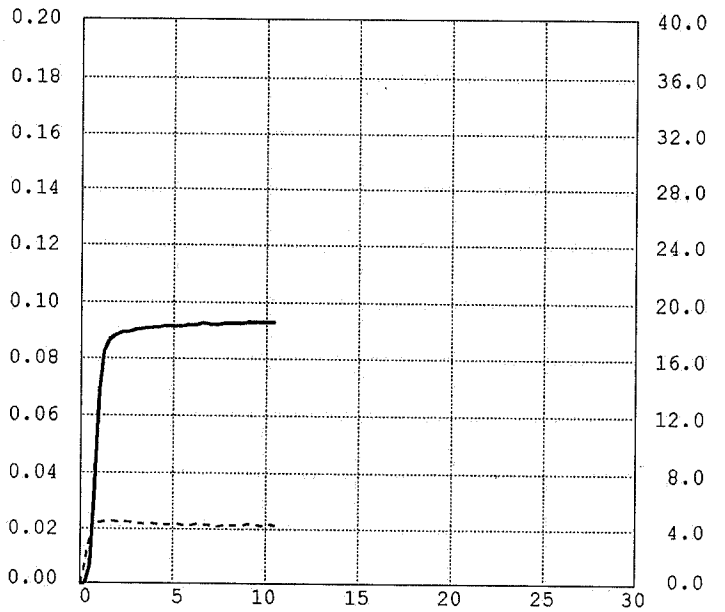

SUPERVISOR TEST




 SUC MORRISVILLE
 UNIVERSITY POLICE
 DATAMASTER dmt: 100123

Date: 01/05/2018

Operator Name: NICOLE M WRIGHT
 Permit #: 41034
 Operator Agency/Dept: SUC MORRISVILLE PD
 Reference Standard #: 17310

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:06
INTERNAL STANDARD	VERIFIED	08:06
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	08:07
BLANK TEST	0.00	08:07
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	08:08
BLANK TEST	0.00	08:08
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	08:09
BLANK TEST	0.00	08:09

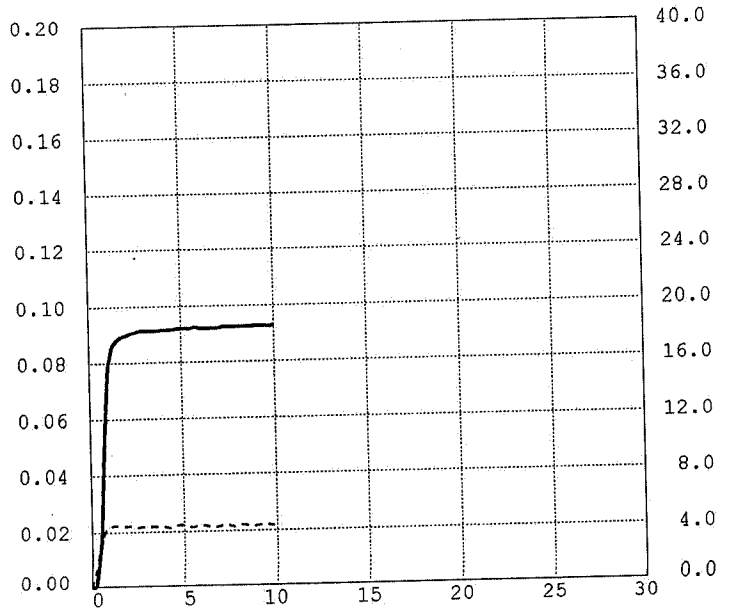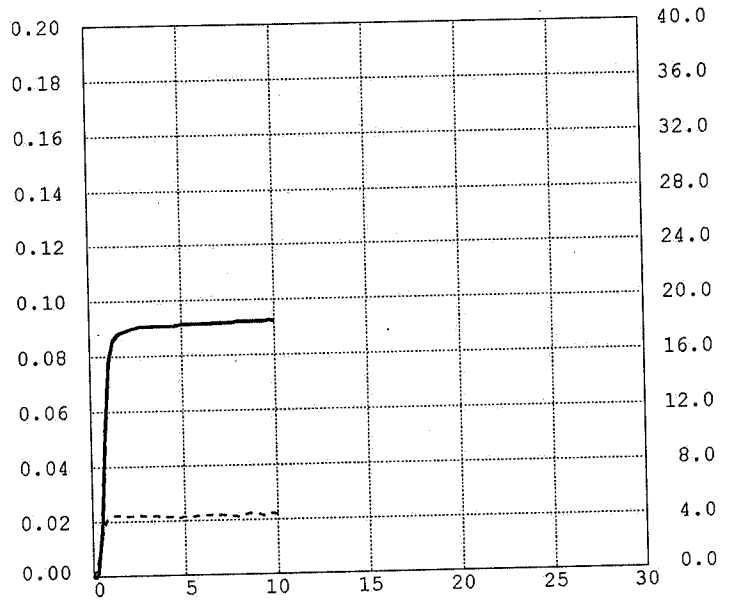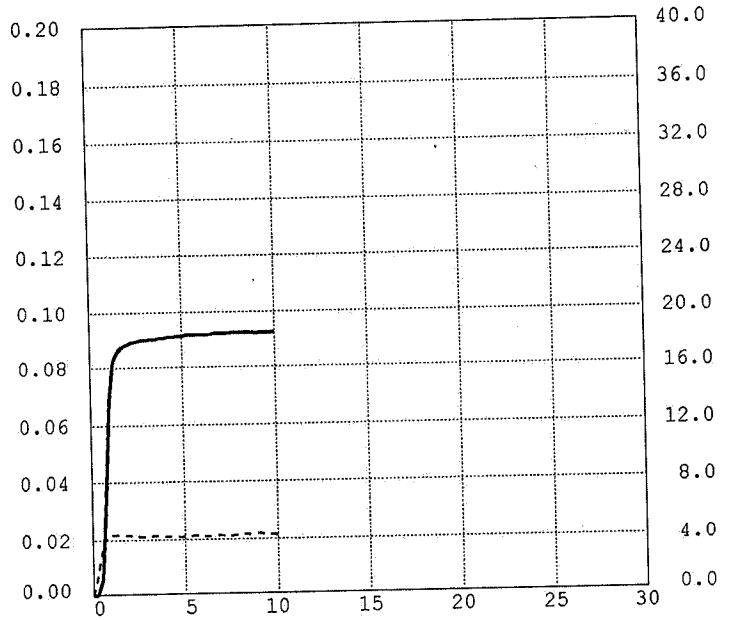

SOLUTION CHANGE

 SUC MORRISVILLE
 UNIVERSITY POLICE
 DATAMASTER dmt: 100123

Date: 01/12/2018

Operator Name: RICHARD P BOWMAN
 Permit #: 44635
 Operator Agency/Dept: SUC MORRISVILLE PD
 Reference Standard #: 17310

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:33
INTERNAL STANDARD	VERIFIED	03:33
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	03:34
BLANK TEST	0.00	03:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:35
BLANK TEST	0.00	03:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:36
BLANK TEST	0.00	03:37

