

**Infrared Instrument
Weekly Calibration Verification Test Record**

Department: NYSOP Morrisville

Instrument Serial #: 100123

Test Date	Simulator Solution Lot #	Simulator Temperature			Sim. Serial#	Test Results			Breath Analysis Supervisor	Sim. Sol. Change *
		1	2	3		1	2	3		
1/6/20	19250	34.00	34.00	34.00	MP4464	.10	.10	.10	MACKO	X
1/10/20	19250	34.00	34.00	33.99	MP4400	.10	.10	.10	MACKO	
1/17/20	19250	33.99	33.99	33.99	MP4400	.10	.10	.10	Wright	
1/25/19	19250	33.99	34.00	34.00	MP4400	.10	.09	.10	Morgan	

* - Please enter a √ to denote simulator solution change taking place

SOLUTION CHANGE




NYS UNIVERSITY POLICE
SUNY MORRISVILLE
DATAMASTER dmt: 100123

Date: 01/06/2020

OPERATOR NAME:
JONATHAN S MACKO
Permit #: 45982
Operator Agency/Dept: SUC MORRISVILLE
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:06
INTERNAL STANDARD	VERIFIED	08:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:07
BLANK TEST	0.00	08:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:08
BLANK TEST	0.00	08:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:09
BLANK TEST	0.00	08:10

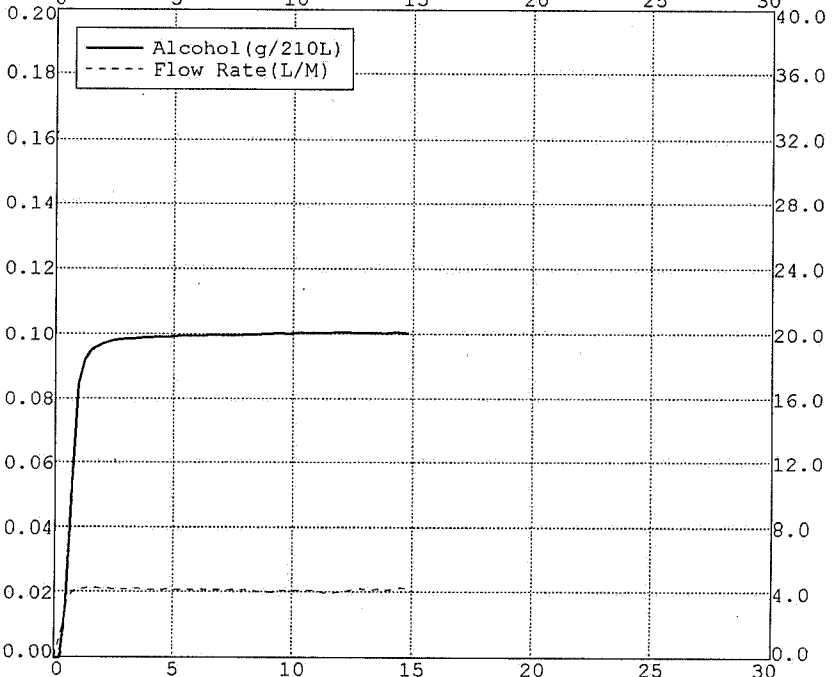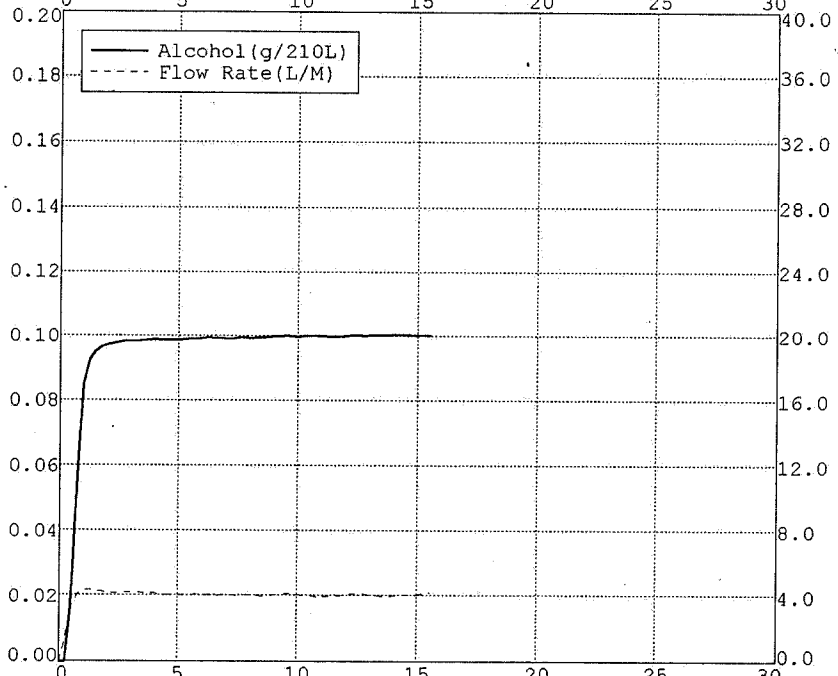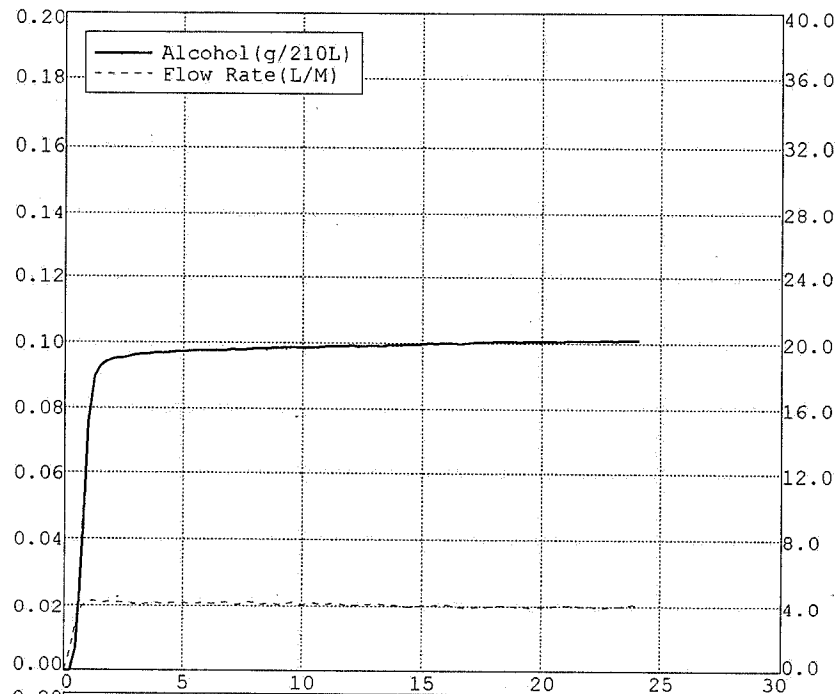

SUPERVISOR TEST




NYS UNIVERSITY POLICE
SUNY MORRISVILLE
DATAMASTER dmt: 100123

Date: 01/10/2020

OPERATOR NAME:
JONATHAN S MACKO
Permit #: 45982
Operator Agency/Dept: SUC MORRISVILLE
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:50
INTERNAL STANDARD	VERIFIED	11:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:50
BLANK TEST	0.00	11:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:51
BLANK TEST	0.00	11:52
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	11:53
BLANK TEST	0.00	11:54

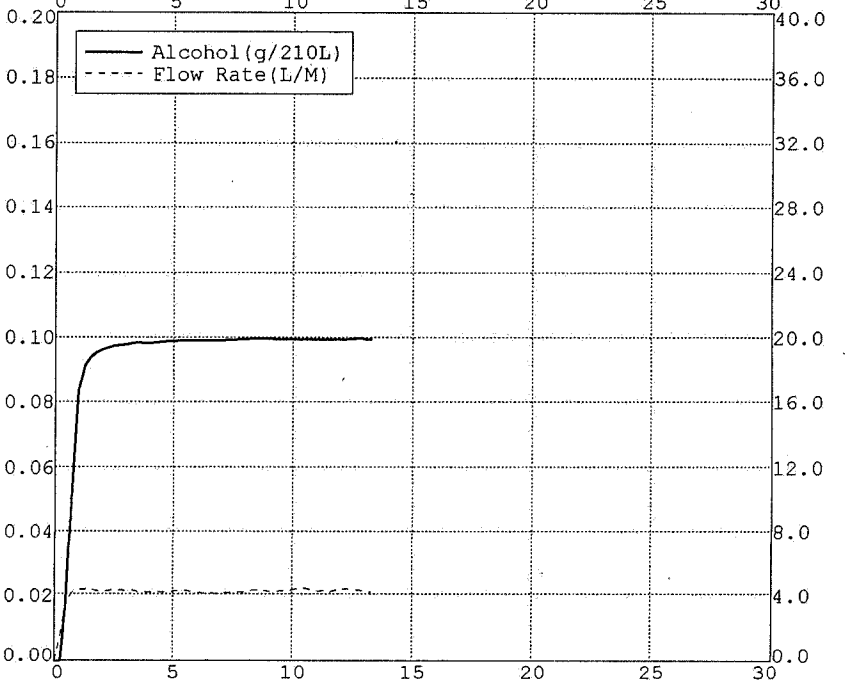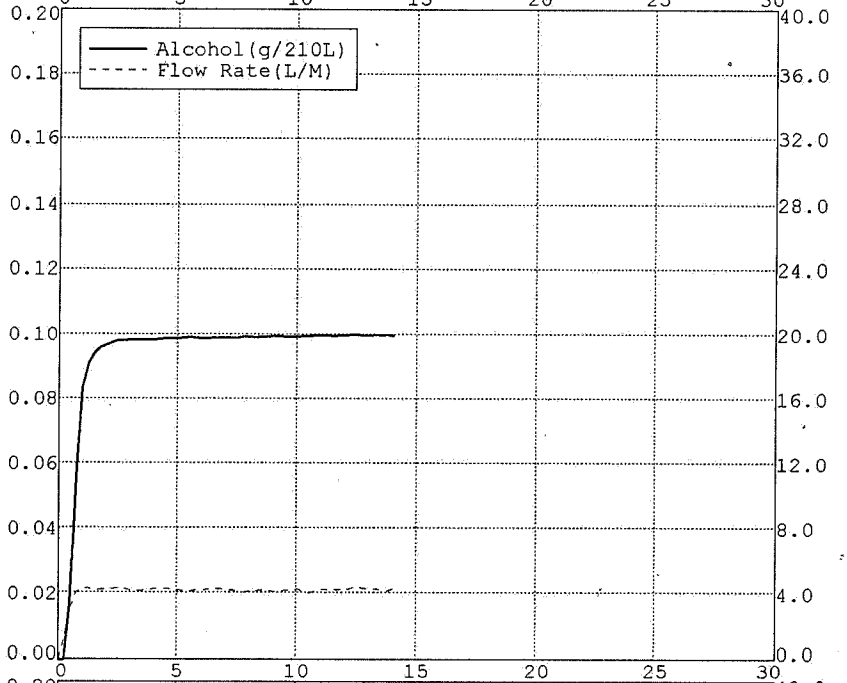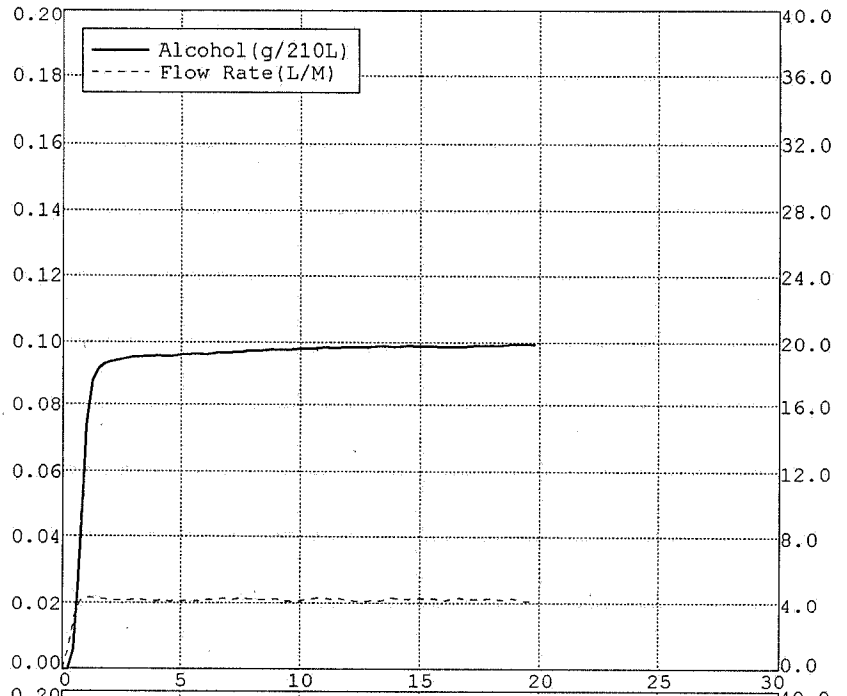

SUPERVISOR TEST




NYS UNIVERSITY POLICE
SUNY MORRISVILLE
DATAMASTER dmt: 100123

Date: 01/17/2020

OPERATOR NAME:
NICOLE M WRIGHT
Permit #: 41034
Operator Agency/Dept: SUC MORRISVILLE
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:47
INTERNAL STANDARD	VERIFIED	14:47
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	14:48
BLANK TEST	0.00	14:49
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	14:49
BLANK TEST	0.00	14:50
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	14:50
BLANK TEST	0.00	14:51

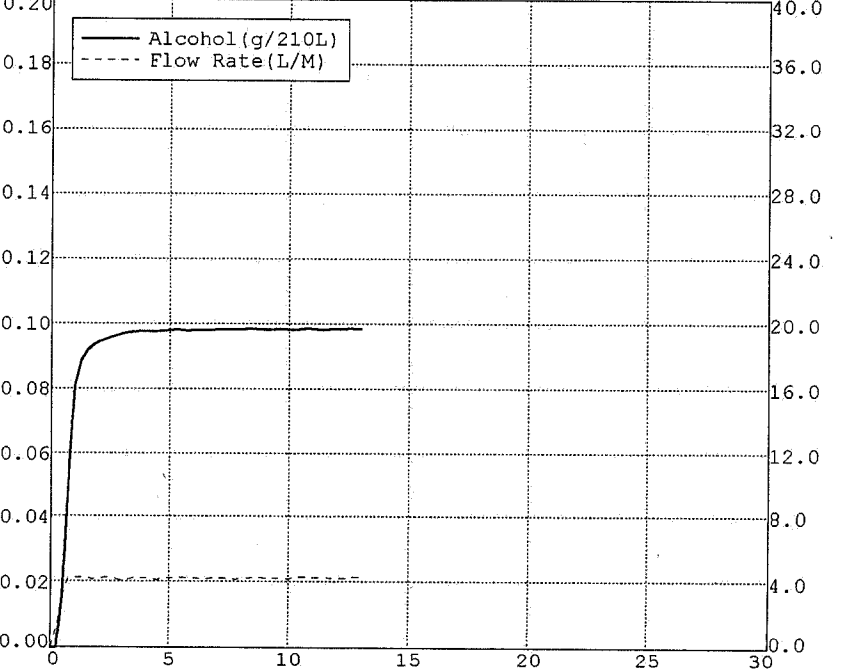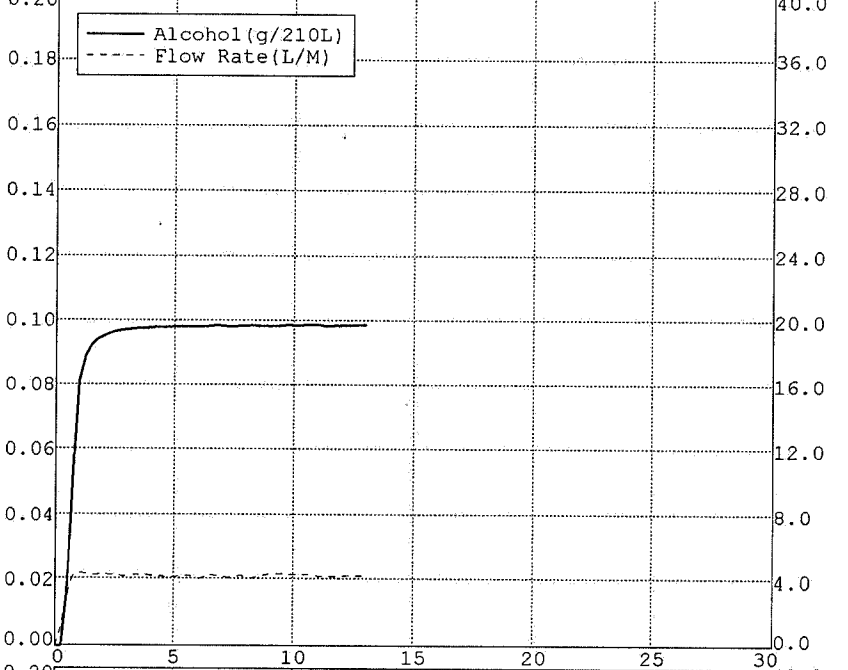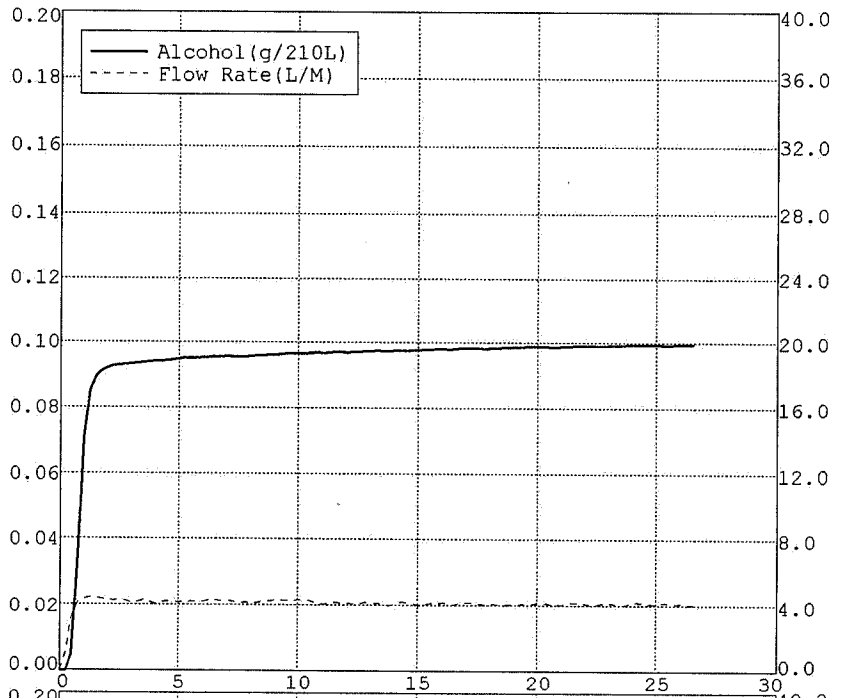

SUPERVISOR TEST

NYS UNIVERSITY POLICE
SUNY MORRISVILLE
DATAMASTER dmt: 100123

Date: 01/25/2020

OPERATOR NAME:
TYLER J MORGAN
Permit #: 45936
Operator Agency/Dept: SUC MORRISVILLE
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:04
INTERNAL STANDARD	VERIFIED	04:04
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	04:05
BLANK TEST	0.00	04:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	04:06
BLANK TEST	0.00	04:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	04:07
BLANK TEST	0.00	04:08

