

SOLUTION CHANGE



ONEIDA CITY
POLICE DEPT
MATAMASTER dmt: 137806

Date: 01/31/2020

OPERATOR NAME:
STEVEN J LOWELL
Permit #: 40046
Operator Agency/Dept: ONEIDA CITY PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:38
INTERNAL STANDARD	VERIFIED	01:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:39
BLANK TEST	0.00	01:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:40
BLANK TEST	0.00	01:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:41
BLANK TEST	0.00	01:42

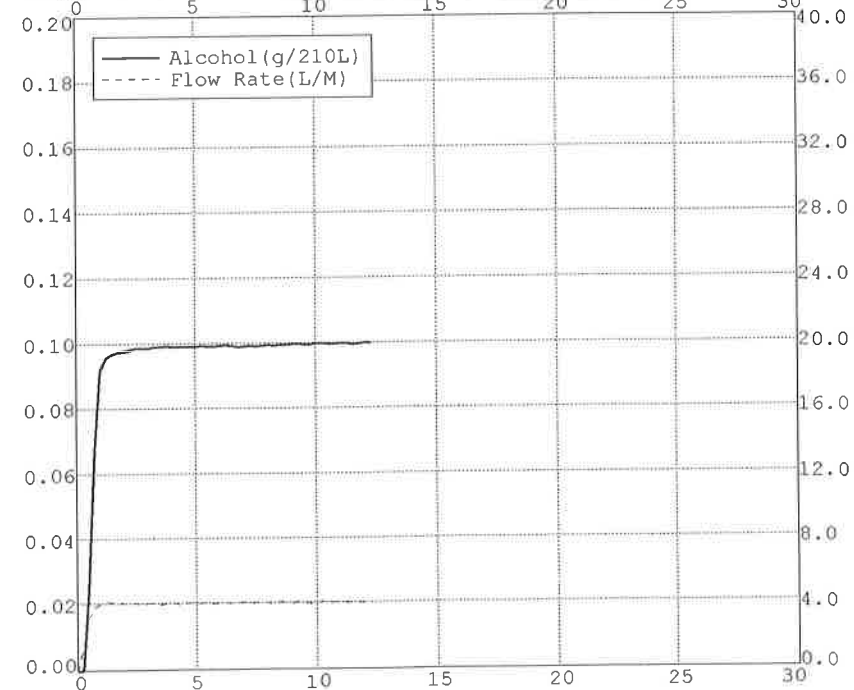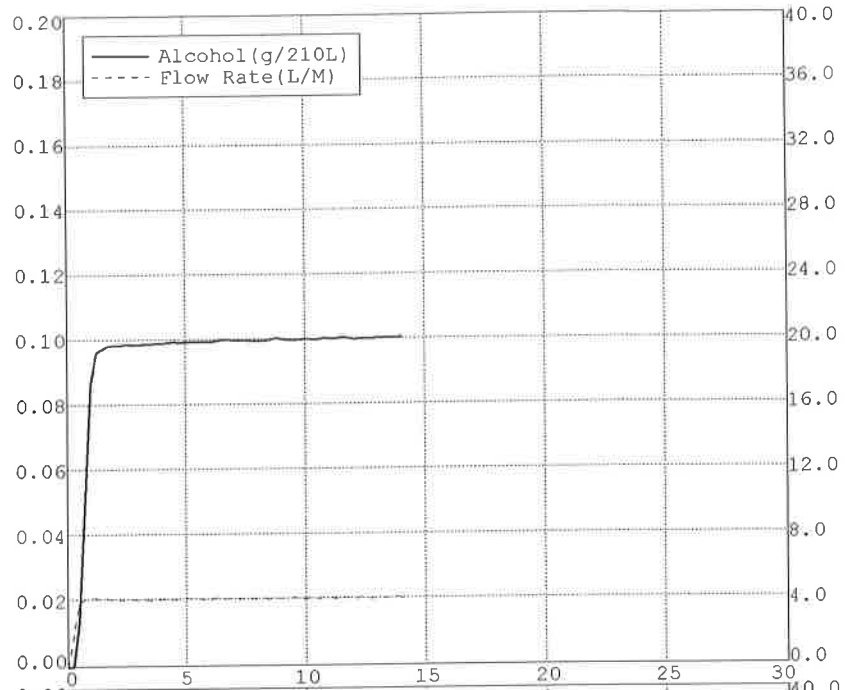

SUPERVISOR TEST




ONEIDA CITY
POLICE DEPT
DATAMASTER dmt: 137806

Date: 01/27/2020

OPERATOR NAME:
STEVEN J LOWELL
Permit #: 40046
Operator Agency/Dept: ONEIDA CITY PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:13
INTERNAL STANDARD	VERIFIED	20:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	20:13
BLANK TEST	0.00	20:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	20:14
BLANK TEST	0.00	20:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	20:15
BLANK TEST	0.00	20:16

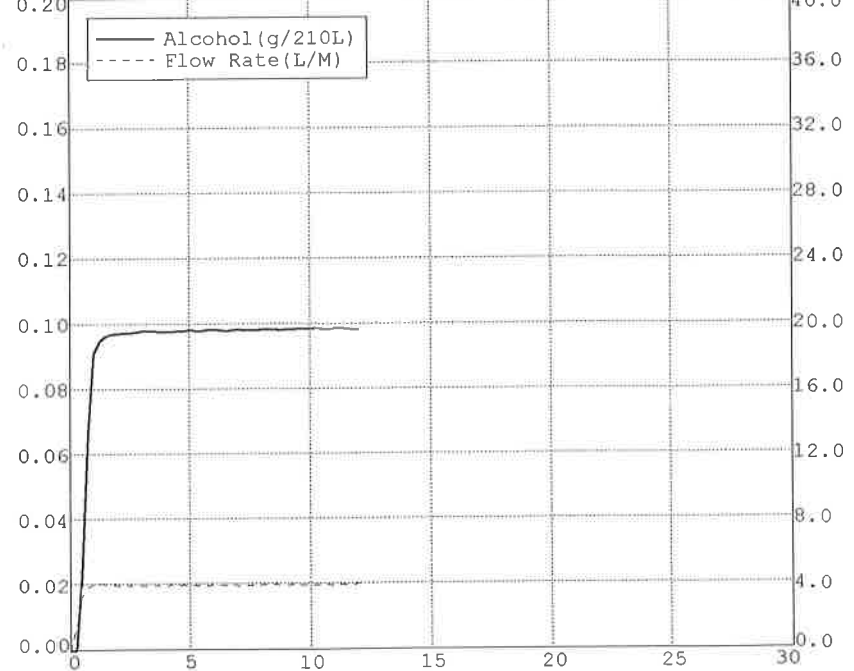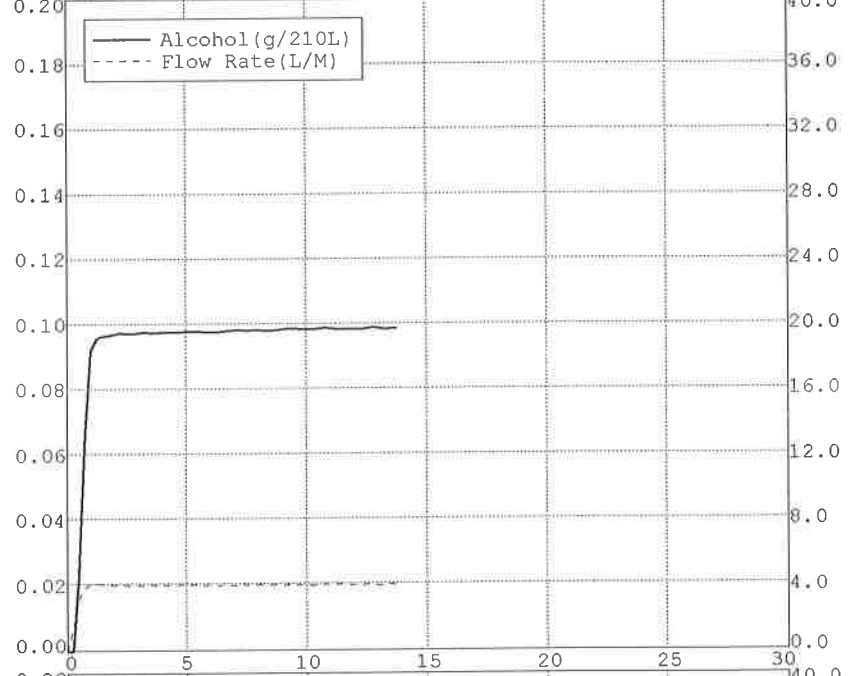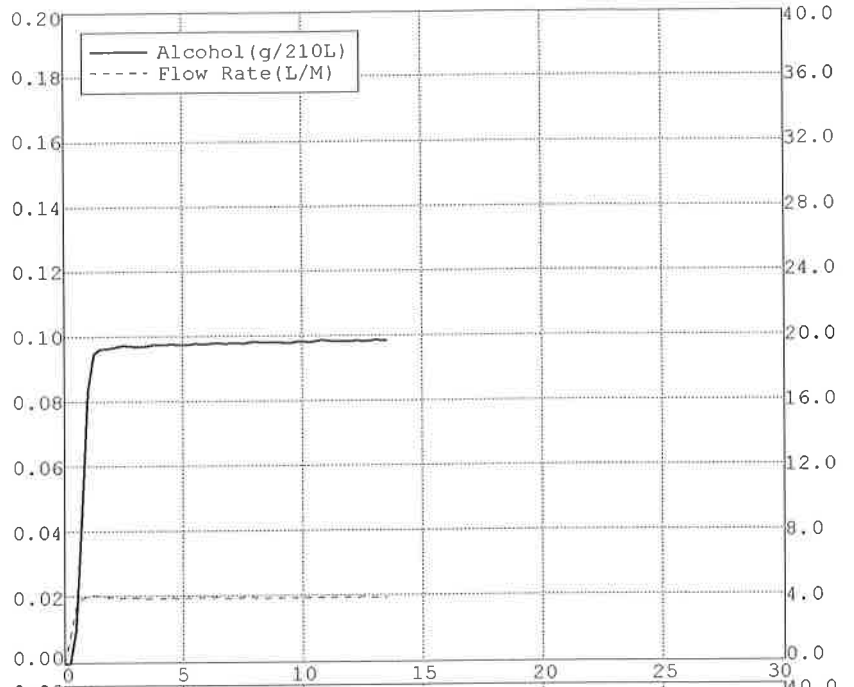

SUPERVISOR TEST


ONEIDA CITY
POLICE DEPT
DATAMASTER dmt: 137806

Date: 01/21/2020

OPERATOR NAME:
STEVEN J LOWELL
Permit #: 40046
Operator Agency/Dept: ONEIDA CITY PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:44
INTERNAL STANDARD	VERIFIED	12:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:44
BLANK TEST	0.00	12:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:45
BLANK TEST	0.00	12:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:46
BLANK TEST	0.00	12:47

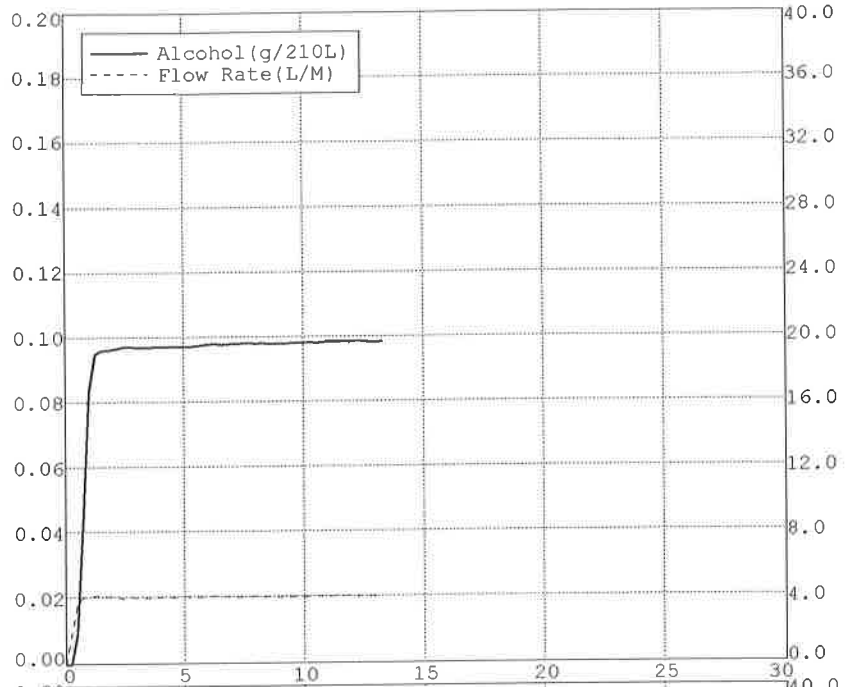

SUPERVISOR TEST



ONEIDA CITY
POLICE DEPT
DATAMASTER dmt: 137806

ate: 01/15/2020

OPERATOR NAME:
STEVEN J LOWELL
Permit #: 40046
Operator Agency/Dept: ONEIDA CITY PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:55
INTERNAL STANDARD	VERIFIED	18:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:55
BLANK TEST	0.00	18:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:56
BLANK TEST	0.00	18:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:57
BLANK TEST	0.00	18:58

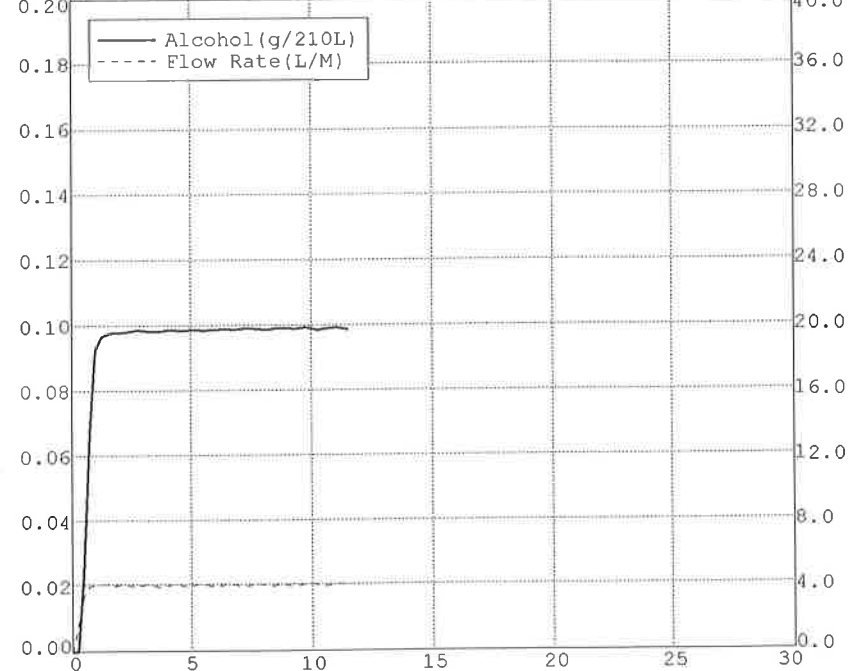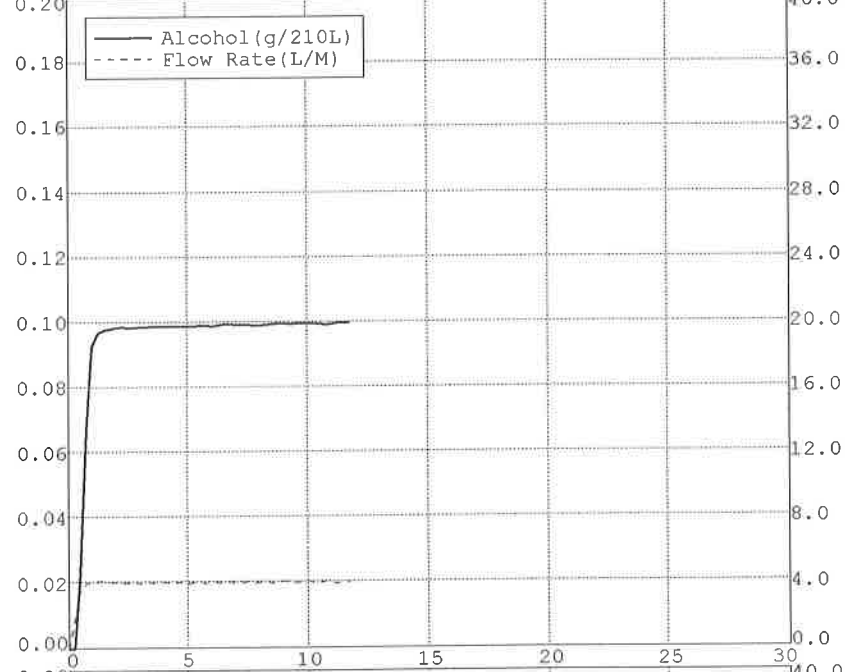

SUPERVISOR TEST




ONEIDA CITY
POLICE DEPT
MATAMASTER dmt: 137806

Date: 01/09/2020

OPERATOR NAME:
STEVEN J LOWELL
Permit #: 40046
Operator Agency/Dept: ONEIDA CITY PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:02
INTERNAL STANDARD	VERIFIED	19:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:03
BLANK TEST	0.00	19:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:04
BLANK TEST	0.00	19:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:05
BLANK TEST	0.00	19:06

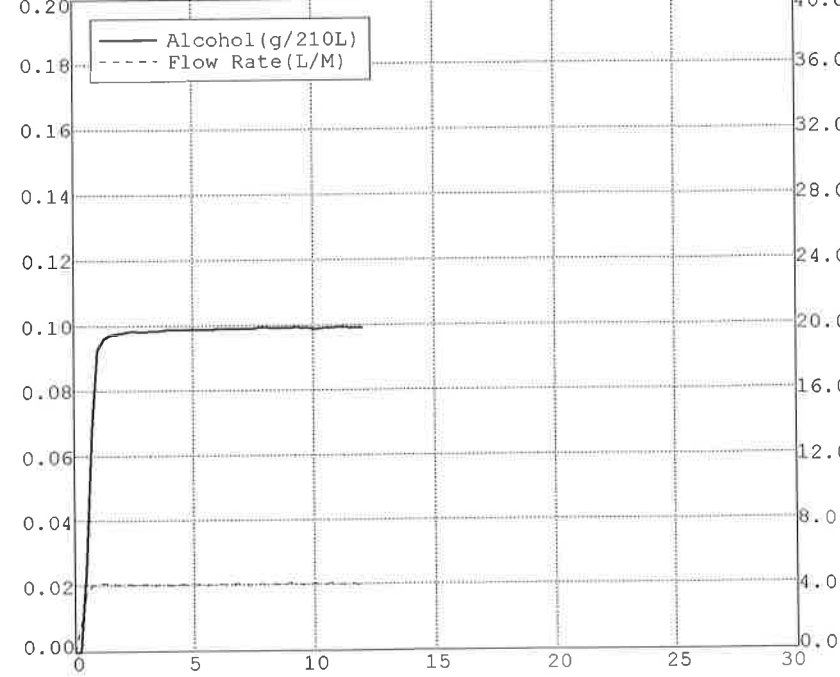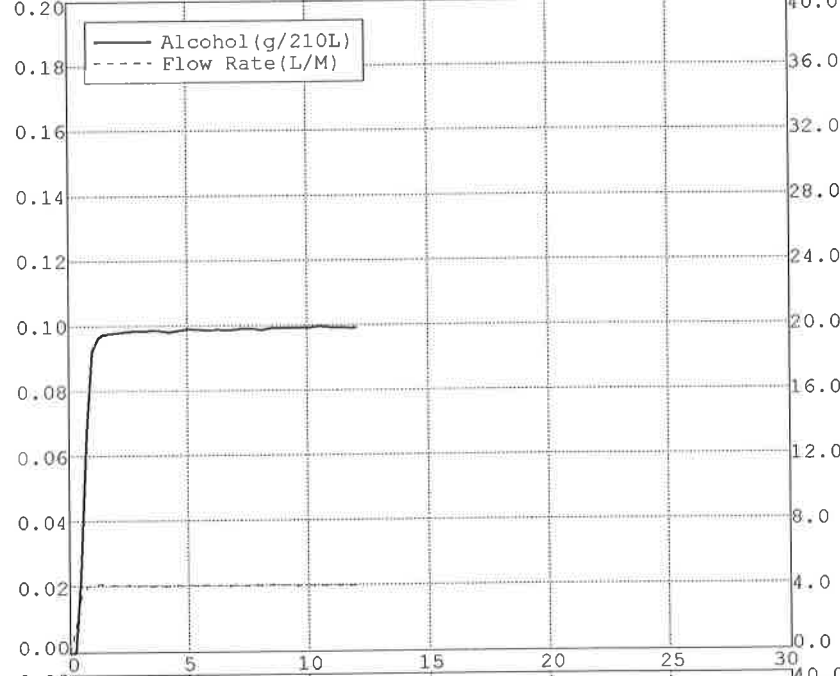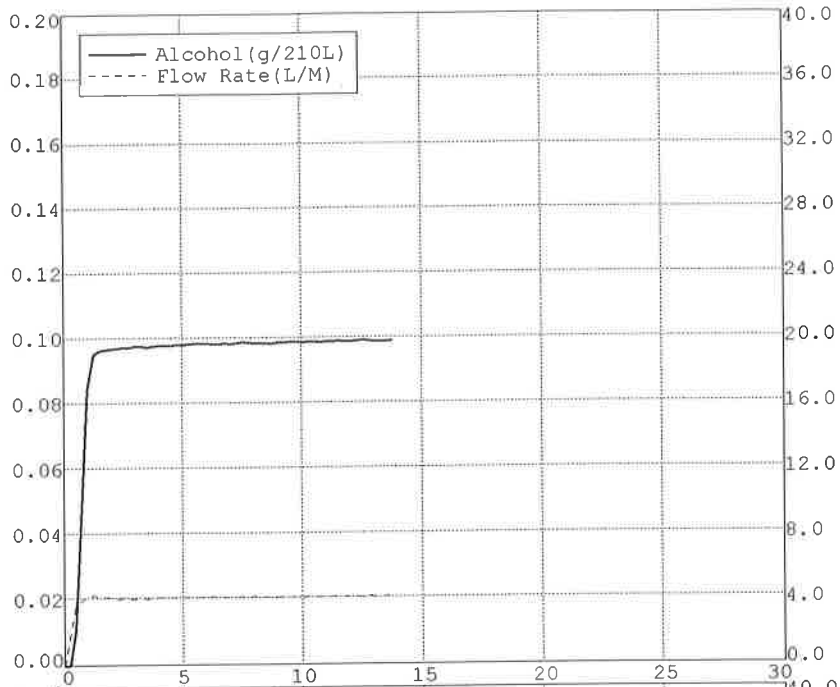

SUPERVISOR TEST




ONEIDA CITY
POLICE DEPT
MATAMASTER dmt: 137806

Date: 01/03/2020

OPERATOR NAME:
STEVEN J LOWELL
Permit #: 40046
Operator Agency/Dept: ONEIDA CITY PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:06
INTERNAL STANDARD	VERIFIED	19:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:07
BLANK TEST	0.00	19:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:08
BLANK TEST	0.00	19:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:09
BLANK TEST	0.00	19:10

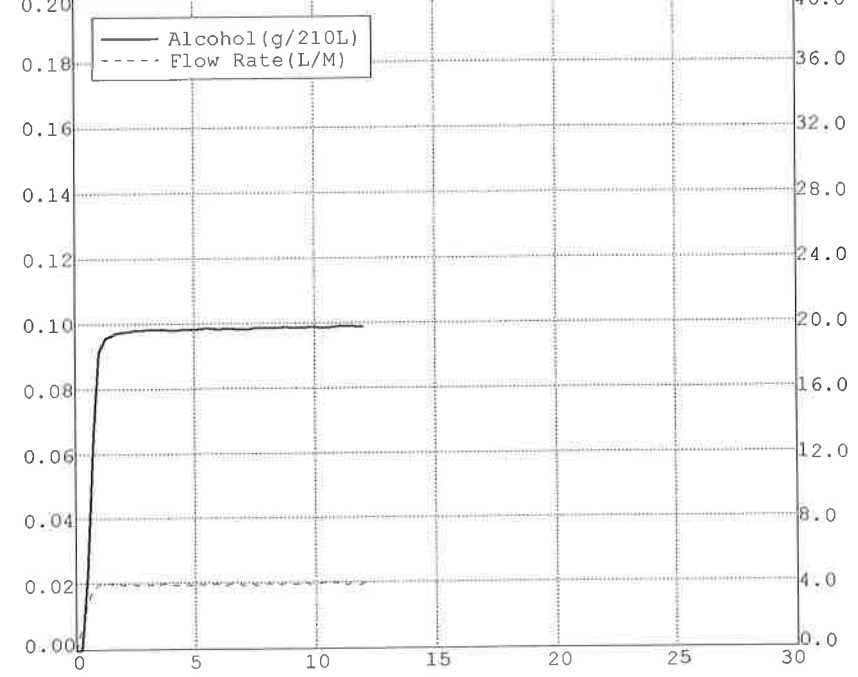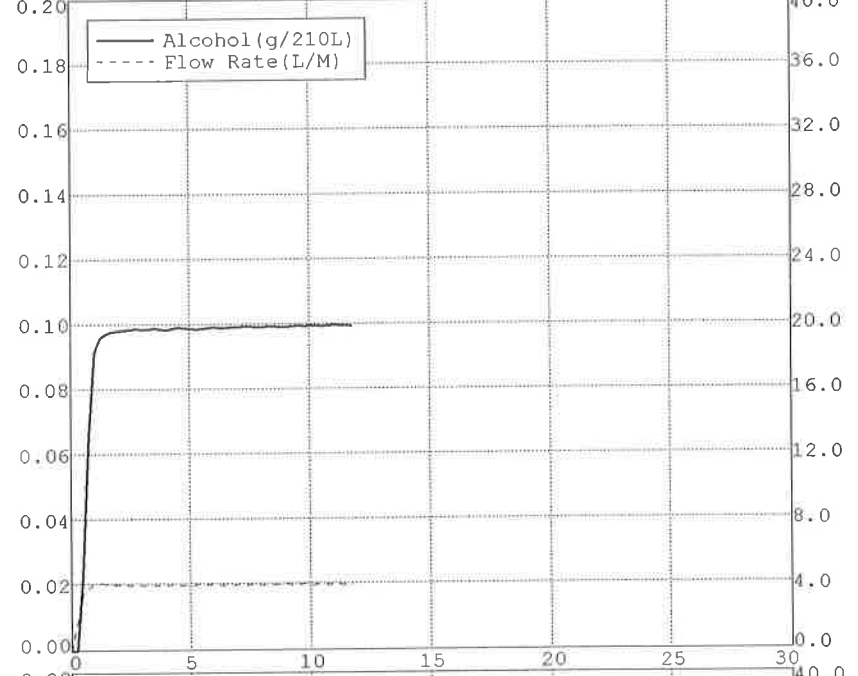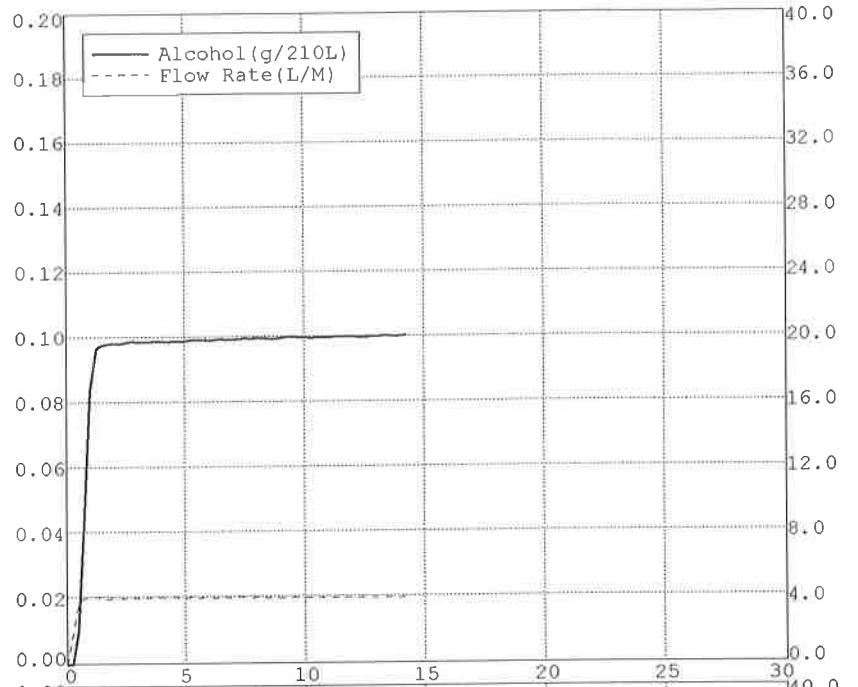

SOLUTION CHANGE

ONEIDA CITY
POLICE DEPT
DATAMASTER dmt: 137806

Date: 12/31/2019

OPERATOR NAME:
STEVEN J LOWELL
Permit #: 40046
Operator Agency/Dept: ONEIDA CITY PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:25
INTERNAL STANDARD	VERIFIED	00:25
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	00:26
BLANK TEST	0.00	00:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:27
BLANK TEST	0.00	00:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:28
BLANK TEST	0.00	00:29

