

**Infrared Instrument  
Weekly Calibration Verification Test Record**

Department: NYSOP Morrisville

Instrument Serial #: 100123

Test Date	Simulator Solution Lot #	Simulator Temperature			Sim. Serial#	Test Results			Breath Analysis Supervisor	Sim. Sol. Change *
		1	2	3		1	2	3		
1/6/20	19250	34.00	34.00	34.00	MP4464	.10	.10	.10	MACKO	X
1/10/20	19250	34.06	34.00	33.99	MP4400	.10	.10	.10	MACKO	
1/17/20	19250	33.99	33.99	33.99	MP4400	.10	.10	.10	Wright	
1/25/20	19250	33.99	34.00	34.00	MP4400	.10	.09	.10	Morgan	
1/31/20	19250	33.99	33.99	34.00	MP4400	.09	.09	.09	Morgan	
1/17/20	19250	33.99	34.00	33.99	MP4400	.10	.10	.10	Netban 1	
2/7/20	19350	34.00	34.00	34.00	MP4400	.10	.10	.10	MACKO	✓

\* - Please enter a ✓ to denote simulator solution change taking place

SOLUTION CHANGE




NYS UNIVERSITY POLICE  
SUNY MORRISVILLE  
DATAMASTER dmt: 100123

Date: 01/06/2020

OPERATOR NAME:  
JONATHAN S MACKO  
Permit #: 45982  
Operator Agency/Dept: SUC MORRISVILLE  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:06
INTERNAL STANDARD	VERIFIED	08:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:07
BLANK TEST	0.00	08:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:08
BLANK TEST	0.00	08:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:09
BLANK TEST	0.00	08:10

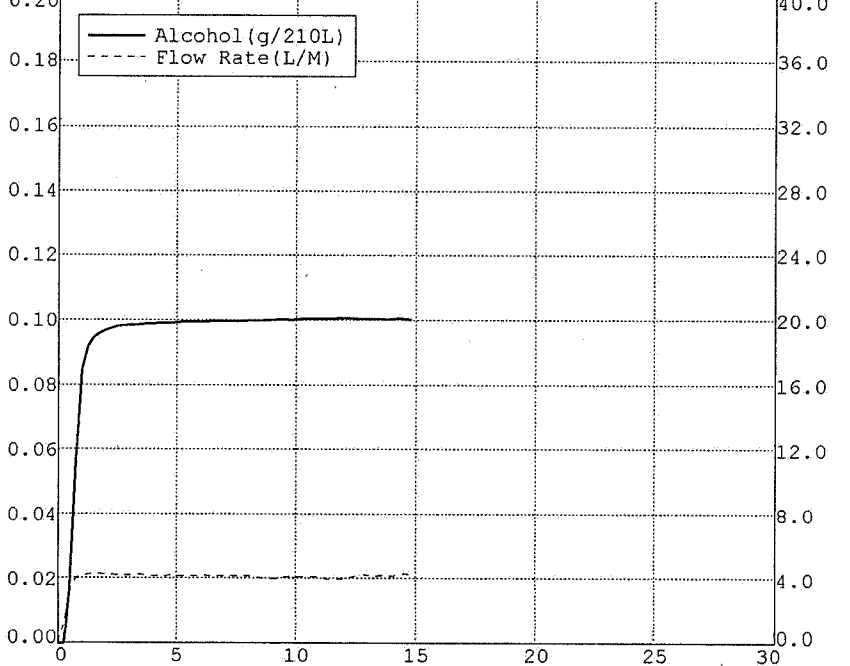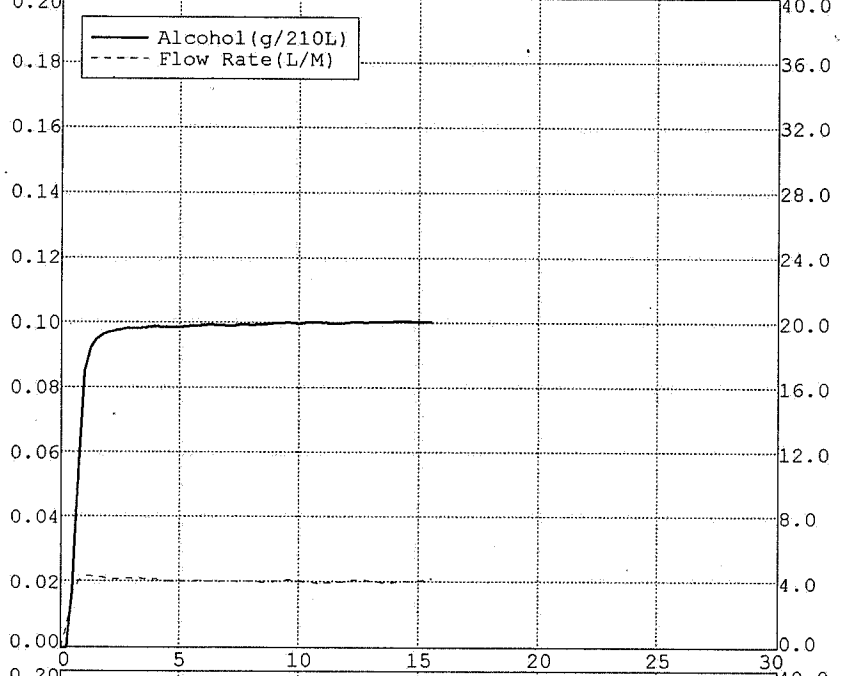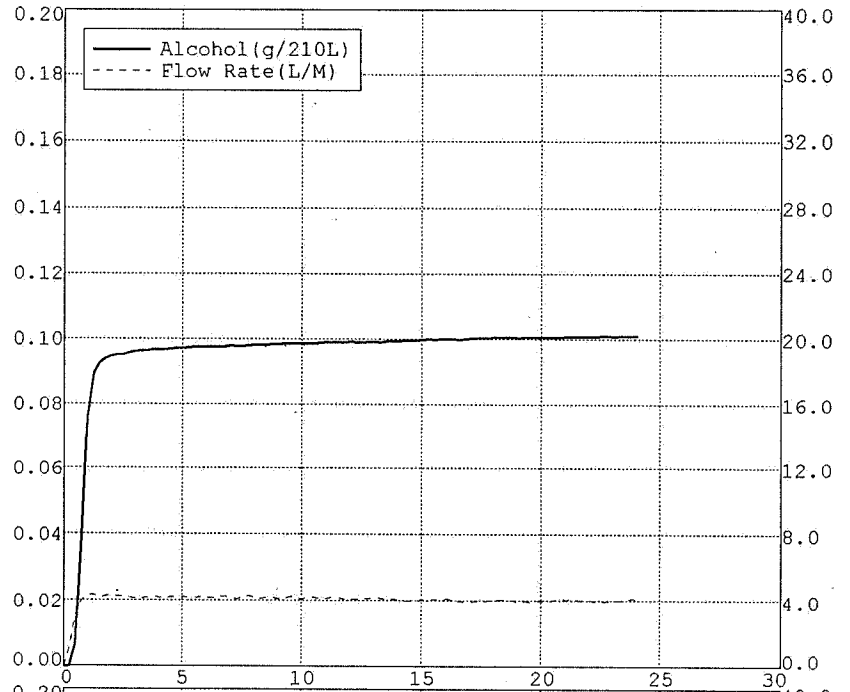

SUPERVISOR TEST




NYS UNIVERSITY POLICE  
SUNY MORRISVILLE  
DATAMASTER dmt: 100123

Date: 01/10/2020

OPERATOR NAME:  
JONATHAN S MACKO  
Permit #: 45982  
Operator Agency/Dept: SUC MORRISVILLE  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:50
INTERNAL STANDARD	VERIFIED	11:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:50
BLANK TEST	0.00	11:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:51
BLANK TEST	0.00	11:52
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	11:53
BLANK TEST	0.00	11:54

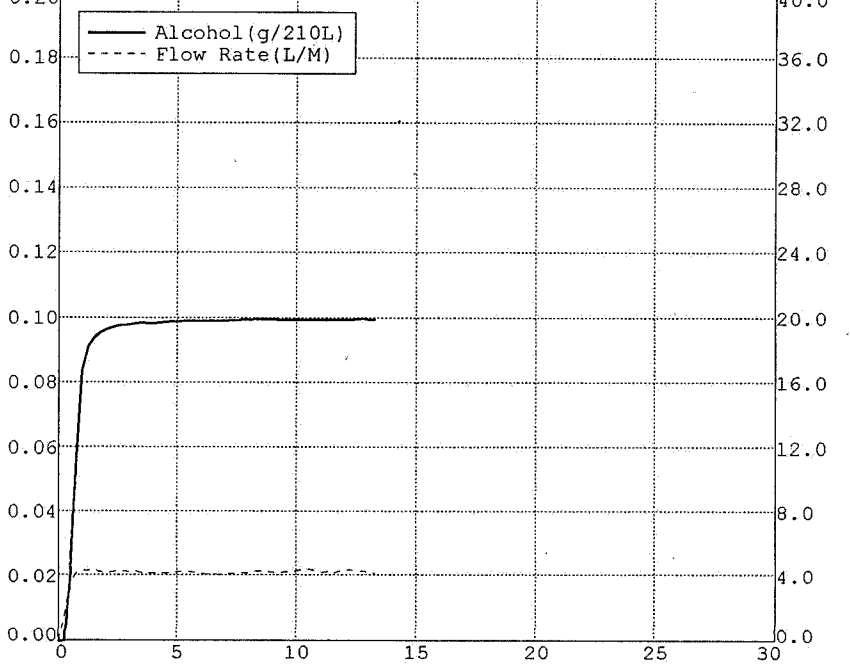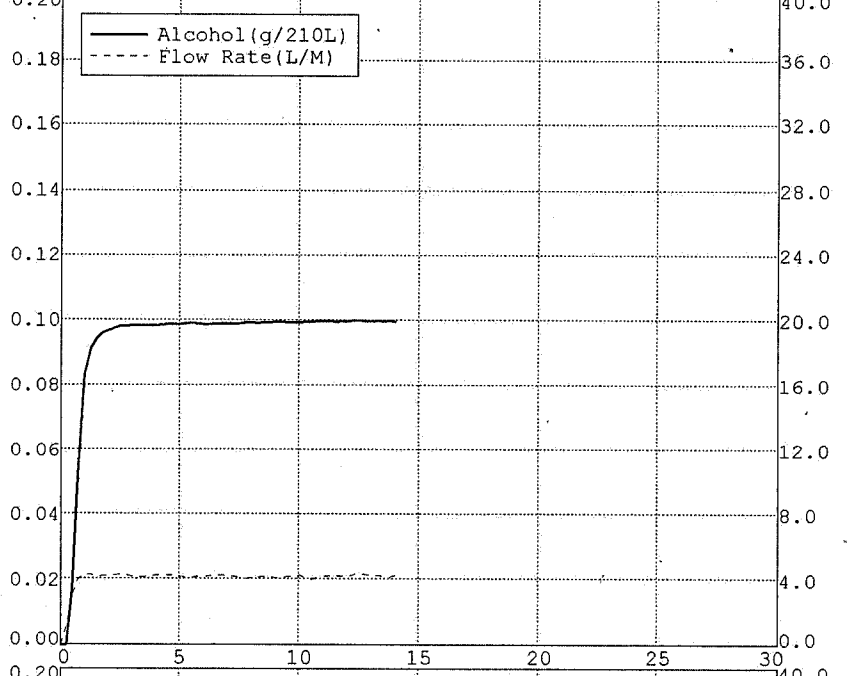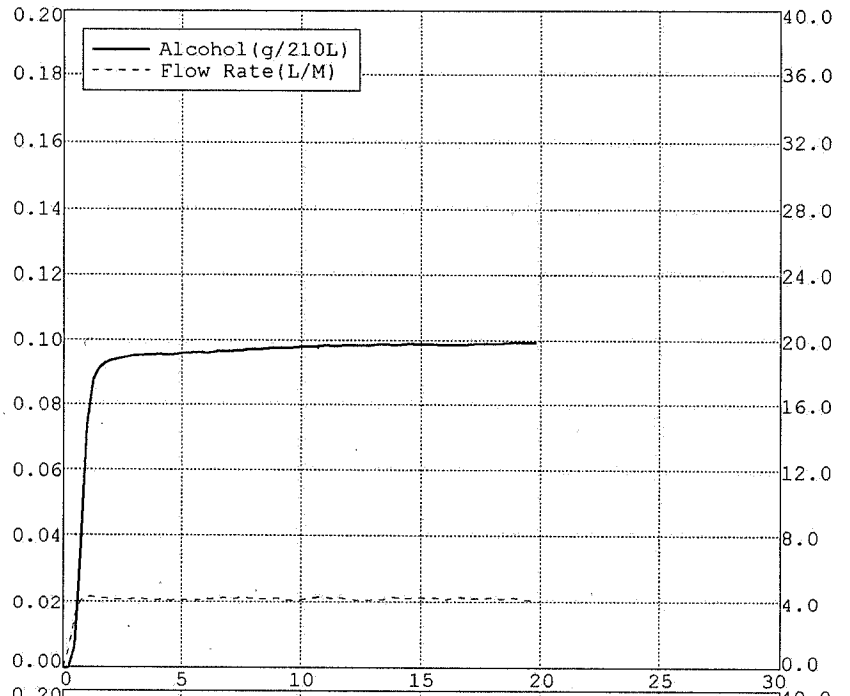

SUPERVISOR TEST




NYS UNIVERSITY POLICE  
SUNY MORRISVILLE  
DATAMASTER dmt: 100123

Date: 01/17/2020

OPERATOR NAME:  
NICOLE M WRIGHT  
Permit #: 41034  
Operator Agency/Dept: SUC MORRISVILLE  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:47
INTERNAL STANDARD	VERIFIED	14:47
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	14:48
BLANK TEST	0.00	14:49
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	14:49
BLANK TEST	0.00	14:50
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	14:50
BLANK TEST	0.00	14:51

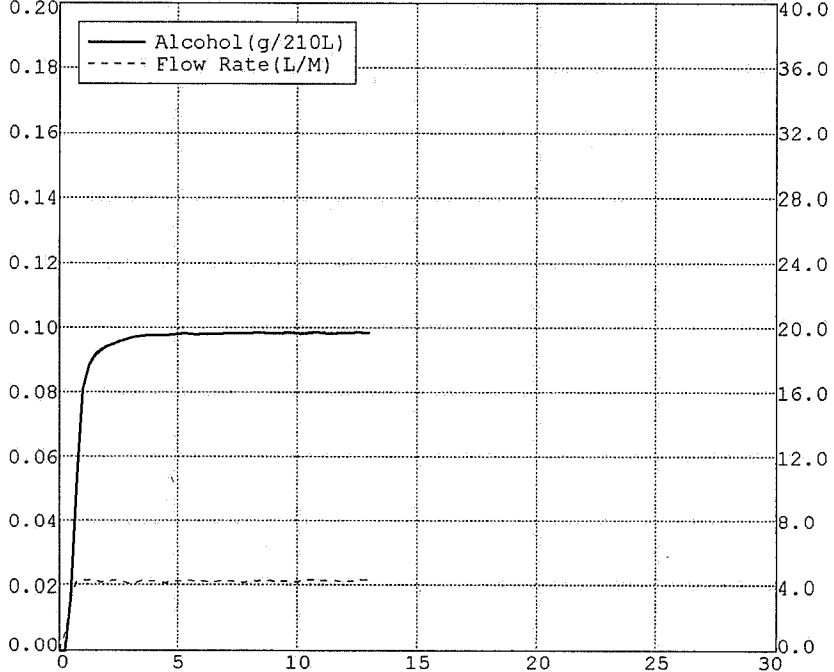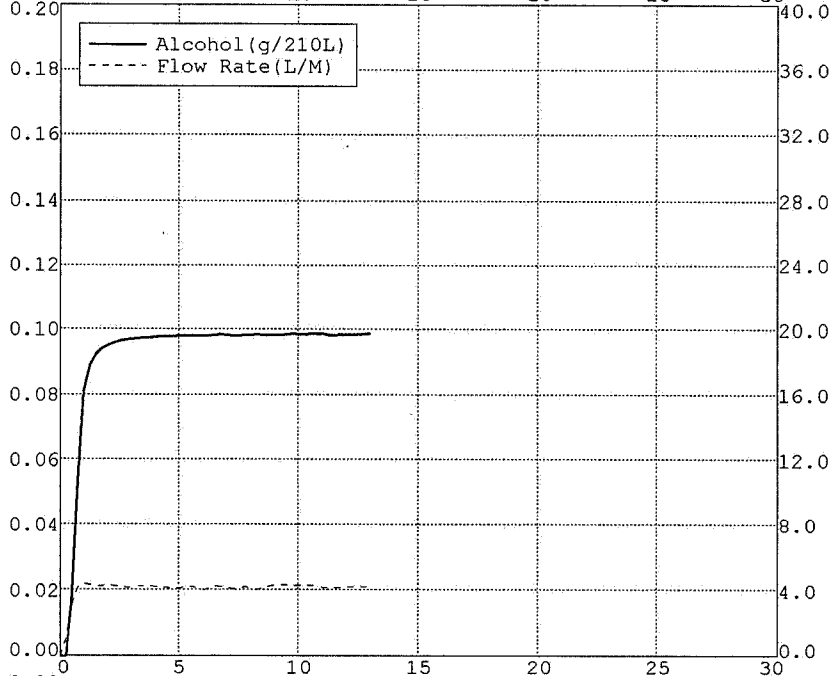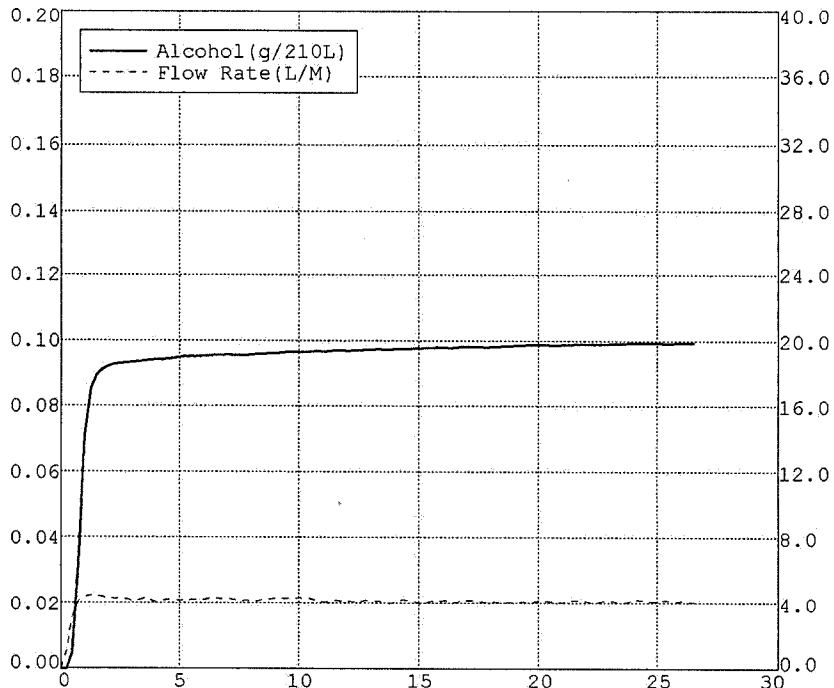

SUPERVISOR TEST




NYS UNIVERSITY POLICE  
SUNY MORRISVILLE  
DATAMASTER dmt: 100123

Date: 01/25/2020

OPERATOR NAME:  
TYLER J MORGAN  
Permit #: 45936  
Operator Agency/Dept: SUC MORRISVILLE  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:04
INTERNAL STANDARD	VERIFIED	04:04
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	04:05
BLANK TEST	0.00	04:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	04:06
BLANK TEST	0.00	04:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	04:07
BLANK TEST	0.00	04:08

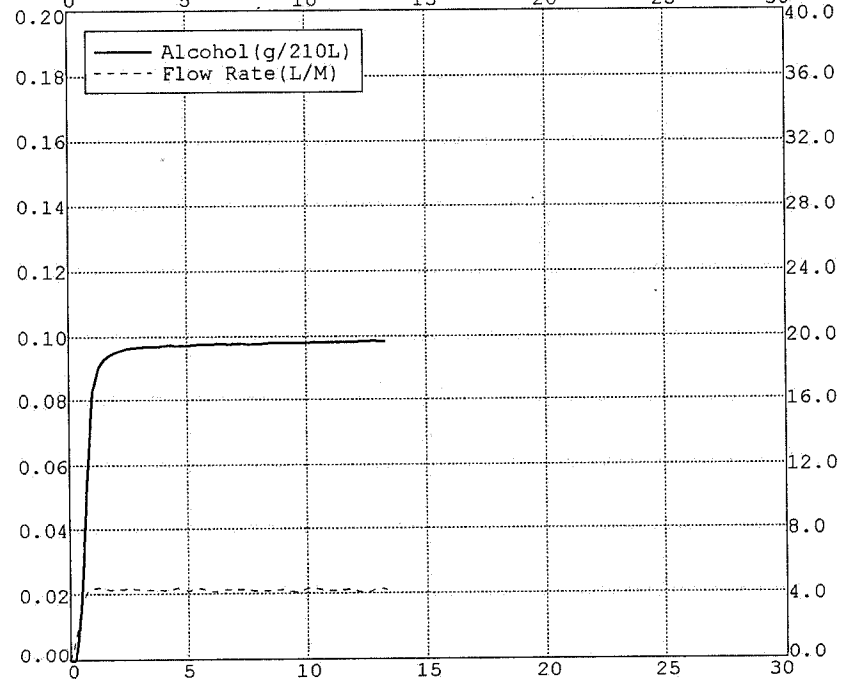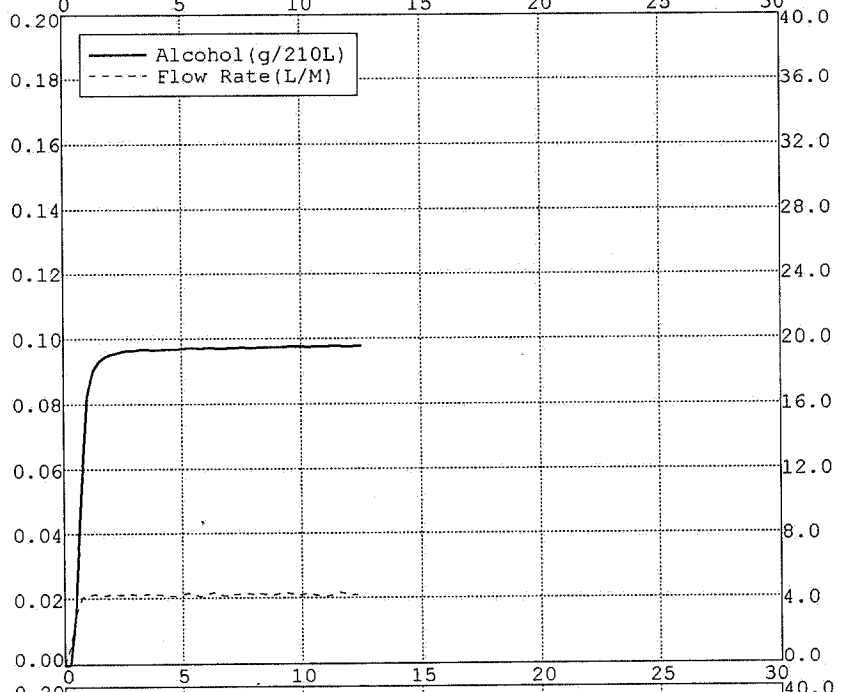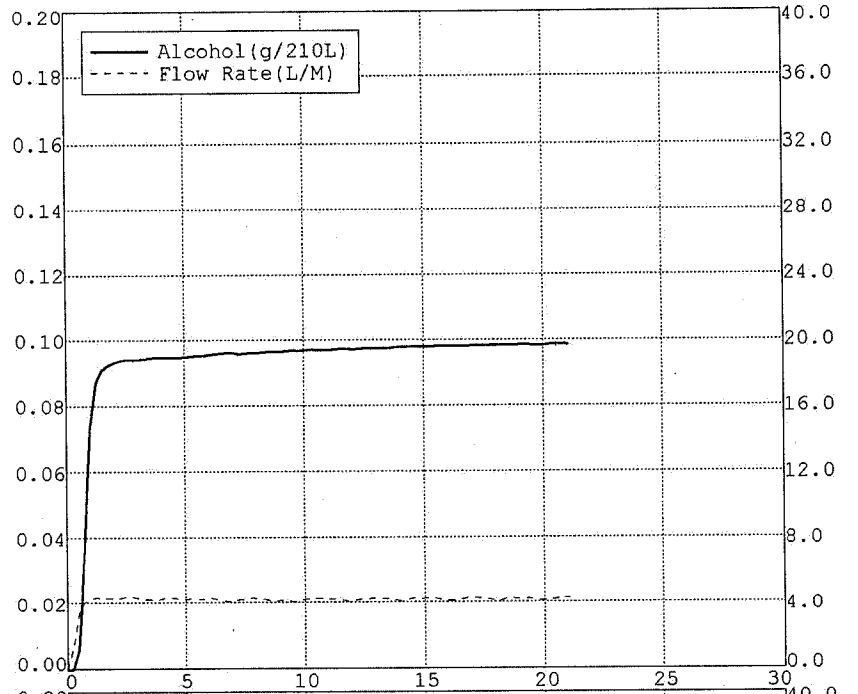

SUPERVISOR TEST



NYS UNIVERSITY POLICE  
SUNY MORRISVILLE  
DATAMASTER dmt: 100123

Date: 01/31/2020

OPERATOR NAME:  
TYLER J MORGAN  
Permit #: 45936  
Operator Agency/Dept: SUC MORRISVILLE  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:37
INTERNAL STANDARD	VERIFIED	06:37
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	06:37
BLANK TEST	0.00	06:38
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	06:39
BLANK TEST	0.00	06:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	06:40
BLANK TEST	0.00	06:41

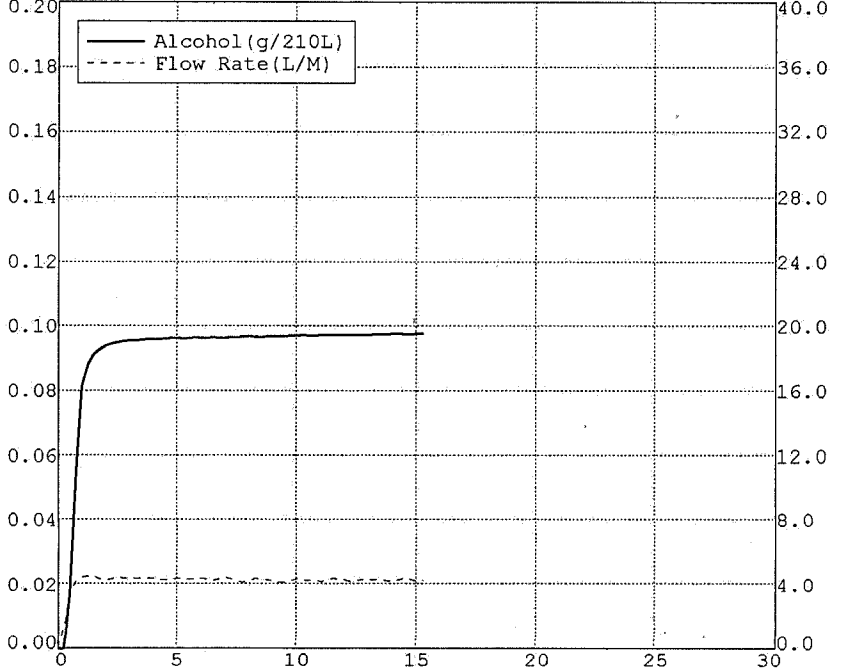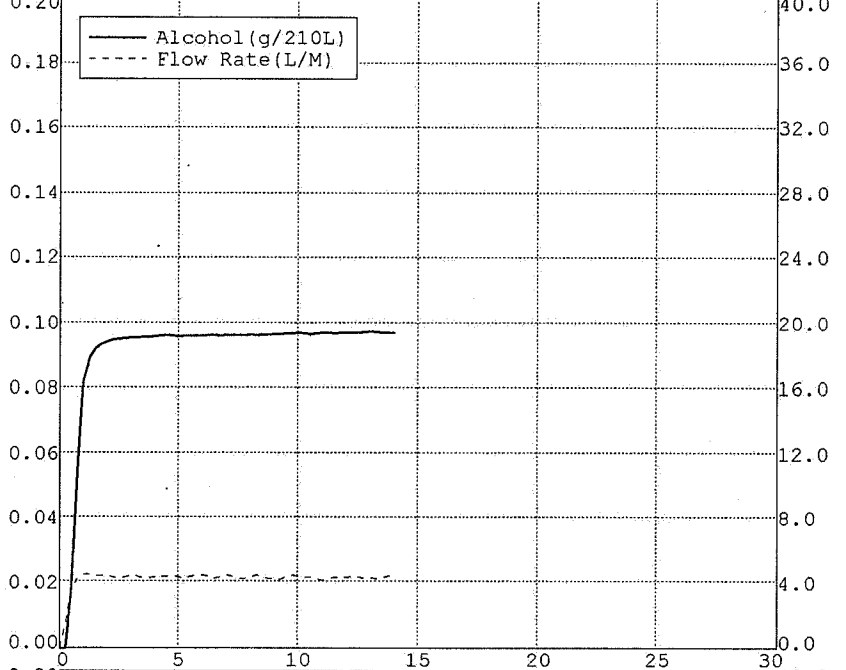

SUPERVISOR TEST




NYS UNIVERSITY POLICE  
 SUNY MORRISVILLE  
 DATAMASTER dmt: 100123

Date: 01/31/2020

OPERATOR NAME:  
 PHILIP B NETZBAND  
 Permit #: 4015  
 Operator Agency/Dept: SUC MORRISVILLE  
 Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:56
INTERNAL STANDARD	VERIFIED	14:56
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	14:56
BLANK TEST	0.00	14:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:58
BLANK TEST	0.00	14:58
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	14:59
BLANK TEST	0.00	15:00

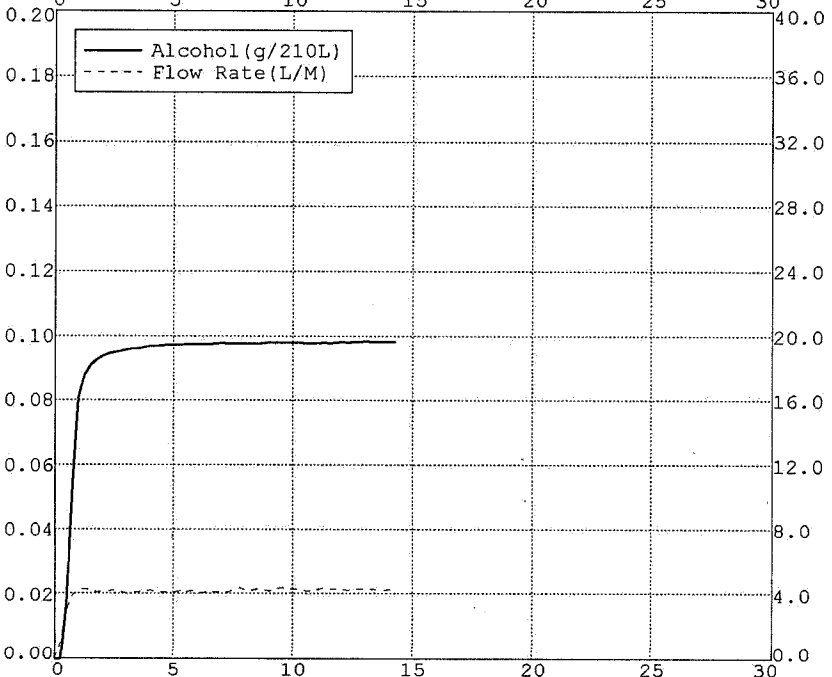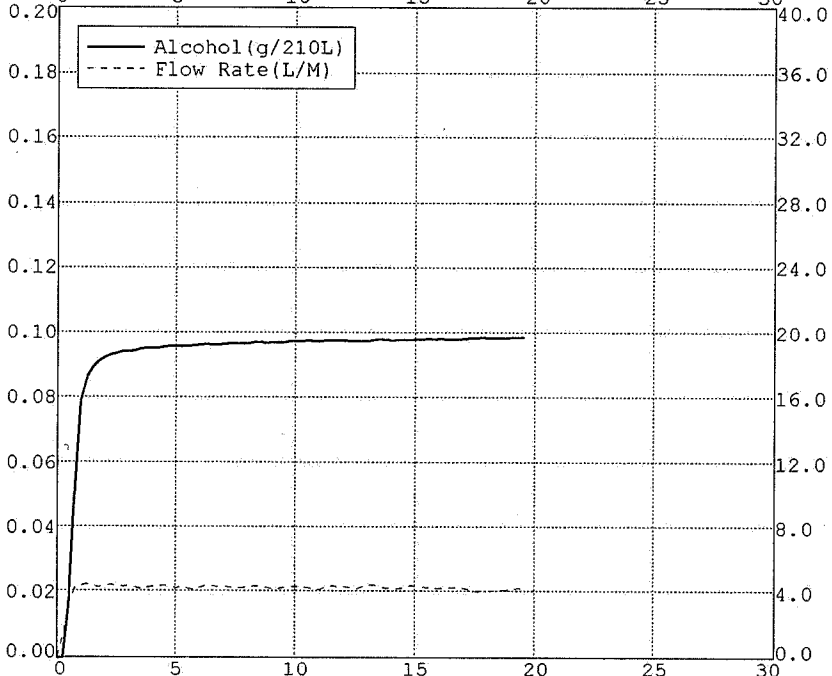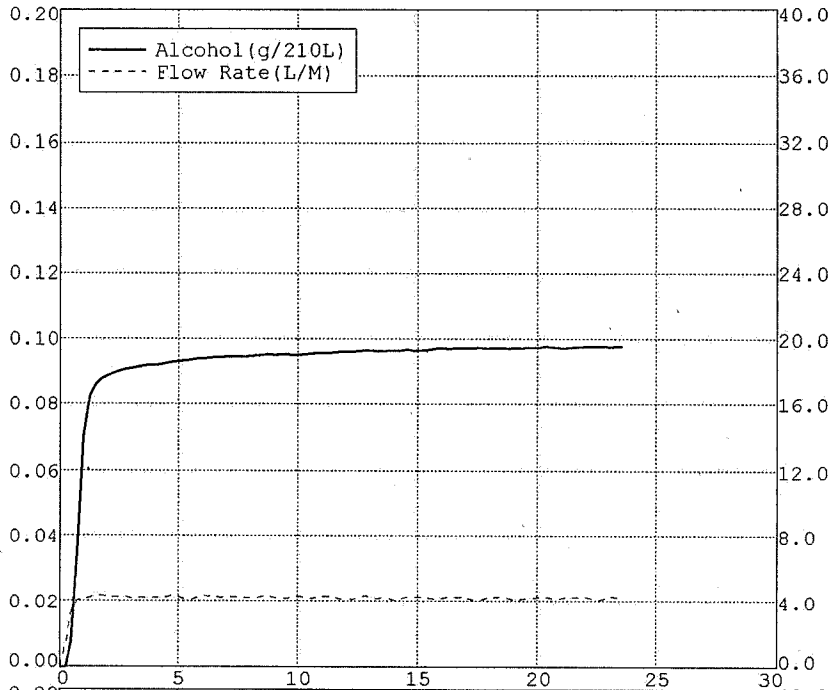

SOLUTION CHANGE

-----  
NYS UNIVERSITY POLICE  
SUNY MORRISVILLE  
DATAMASTER dmt: 100123  
-----

Date: 02/07/2020

OPERATOR NAME:  
JONATHAN S MACKO  
Permit #: 45982  
Operator Agency/Dept: SUC MORRISVILLE  
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:08
INTERNAL STANDARD	VERIFIED	09:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:08
BLANK TEST	0.00	09:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:09
BLANK TEST	0.00	09:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:11
BLANK TEST	0.00	09:11

