

Technical & Administrative Review Checklist - Simulator Solution

Class: Form
ID: Breath Form 4b (Version 5)

Effective Date: January 11, 2017
Page: 1 of 1

Solution Lot Number: 17390

Review Start Date: 12/19/17

Reviewer (initials): CA

Documentation:

- ☒ Handwritten initials on all pages
- ☒ Page number on all pages, total pages noted
- ☒ Solution lot number and bottle number on all solution pages
- ☒ Proper sample loading documented
- ☒ All pages of the technical record were reviewed for corrections; if applicable, corrections were documented appropriately
- ☒ Dates of analyses documented
- ☒ If abbreviations/symbols specific to the laboratory are used, they have been defined in section procedures
- NA Any deviations/departures from acceptability criteria have documented approval

Quality Control Data:

- ☒ Correct version of the test method is indicated on the QC Worksheet
- ☒ Required control samples analyzed, expiration dates not exceeded
- ☒ Acceptance criteria met
- ☒ QC results are accurately entered in Tox Form 11 QC Spreadsheet

Technical Data:

- ☒ The technical records demonstrate compliance with test methods
- ☒ Data transfers are accurate
- ☒ Retention times are recorded and acceptable
- ☒ Results meet acceptability criteria

Simulator Solution Record (electronic):

- ☒ Solution specific information is accurate (e.g. lot number, expiration date, etc)
- ☒ Results are accurately reported
- ☒ Electronic signature applied
- ☒ File name accurate

Review Completed:

- ☒ Upon review of the technical records available, I independently reached the same conclusion(s) reported.

Reviewer (initial/date):

CA 12/19/17
Page 1 of 1

**New York State Police Crime Laboratory System
BREATH TESTING**

Simulator Solution Verification Results

Class: Form

Effective Date: June 1, 2015

ID: Breath Form 2 (Version 3)

Page: 1 of 1

Simulator Solution Level: 0.10 %

Target Concentration: 0.121 %

Acceptable Range: 0.117-0.125 %

Manufacturer: Guth Laboratories, Inc.

Analyst: Carol S Miller

Lot Number: 17390

Analysis Date: 12/19/2017

Bottle Number	% by wt	AVG
6	0.1207 0.1196 0.1198	0.1200
7	0.1202 0.1203 0.1201	0.1202
707	0.1204 0.1205 0.1205	0.1205
708	0.1204 0.1207 0.1206	0.1206
1392	0.1205 0.1208 0.1209	0.1207
1393	0.1212 0.1207 0.1202	0.1207
Grand Average		0.1204

pg 1 of 57 Gem

Approved By: Top Management

Print Date:

12/19/2017

New York State Police Crime Laboratory System

BREATH TESTING

Simulator Solution Verification QC Worksheet

Class: Form
ID: Breath Form 8 (Version 2)

Effective Date: January 10, 2017
Page: 1 of 1

Analysis Date: 12-19-17
Analyst Initials: cm

Breath Instr 2 Version 5

Simulator Solution Lot# 17390

Expiration Date 05-27-18
Received Date 12-07-17
Level 0.10%
Bottle Number(s) 6, 7, 707, 708, 1392, 1393

<u>Internal Standard</u>	<u>Lot #</u>	<u>Expiration Date</u>
n-propanol	<u>AMC120517</u>	<u>03-05-18</u>

<u>Controls</u>	<u>Lot #</u>	<u>Expiration Date</u>
0.08 % by wt	<u>FN10281510</u>	<u>11/2020</u>
0.10 % by wt	<u>FN08101601</u>	<u>08/2021</u>
0.20 % by wt	<u>FN03301601</u>	<u>04/2021</u>
0.30 % by wt	<u>NA</u>	<u>NA</u>
0.40 % by wt	<u>NA</u>	<u>NA</u>
0.50 % by wt	<u>NA</u>	<u>NA</u>
Composite	<u>KMM102317</u>	<u>10-23-18</u>

<u>Instrumentation</u>	<u>Instrument ID/Serial #</u>	<u>Calibration Exp Date</u>
Headspace GC	<u>H TX - HS2</u>	<u>03-05-18</u>
Dilutor	<u>MD916 JE1022</u>	<u>03-31-18</u>

Test Method Analyst Review

Batch Accepted ☒ Batch Rejected ☐

Rejection reason/course of action: _____

Deviations/departures: _____

Comments: _____

Initial/Date: cm 12-19-17

2 cm

Approved By: Top Management

Print Date: 12/19/2017

TotalChrom Sequence File C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

Printed by : manager on: 12/19/2017 7:35:34 AM
Created by : toxicology on: 8/6/2009 1:12:05 PM
Edited by : manager on: 12/19/2017 7:35:31 AM
Number of Times Edited : 51

Description:

Sequence File Header Information:

Number of Rows : 27
Instrument Type : PE AutoSystem GC
Injection Type : SINGLE
Raw tokens channel A :
Result tokens channel A :
Modified tokens channel A :
Raw tokens channel B :
Result tokens channel B :
Modified tokens channel B :

Sequence Sample Descriptions - Channel A

Row	Type	Name
✓1	Sample	COMPOSITE ✓
✓2	Sample	0.08% CONTROL ✓
✓3	Sample	0.10% CONTROL ✓
✓4	Sample	NEG CONTROL ✓
✓5	Sample	GUTH 17390 #6 ✓
✓6	Sample	GUTH 17390 #6 ✓
✓7	Sample	GUTH 17390 #6 ✓
✓8	Sample	GUTH 17390 #7 ✓
✓9	Sample	GUTH 17390 #7 ✓
✓10	Sample	GUTH 17390 #7 ✓
✓11	Sample	GUTH 17390 #707 ✓
✓12	Sample	GUTH 17390 #707 ✓
✓13	Sample	GUTH 17390 #707 ✓
✓14	Sample	0.10% CONTROL ✓
✓15	Sample	NEG CONTROL ✓
✓16	Sample	GUTH 17390 #708 ✓
✓17	Sample	GUTH 17390 #708 ✓
✓18	Sample	GUTH 17390 #708 ✓
✓19	Sample	GUTH 17390 #1392 ✓
✓20	Sample	GUTH 17390 #1392 ✓
✓21	Sample	GUTH 17390 #1392 ✓
✓22	Sample	GUTH 17390 #1393 ✓
✓23	Sample	GUTH 17390 #1393 ✓
✓24	Sample	GUTH 17390 #1393 ✓
✓25	Sample	0.10% CONTROL ✓
✓26	Sample	0.20% CONTROL ✓
✓27	Sample	NEG CONTROL ✓

com
12-19-17


GG
12/19/17

3 com

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36834
Sample Name : COMPOSITE
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 1

Date : 12/19/2017 9:10:38 AM
Data Acquisition Time : 12/19/2017 9:06:12 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-001.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

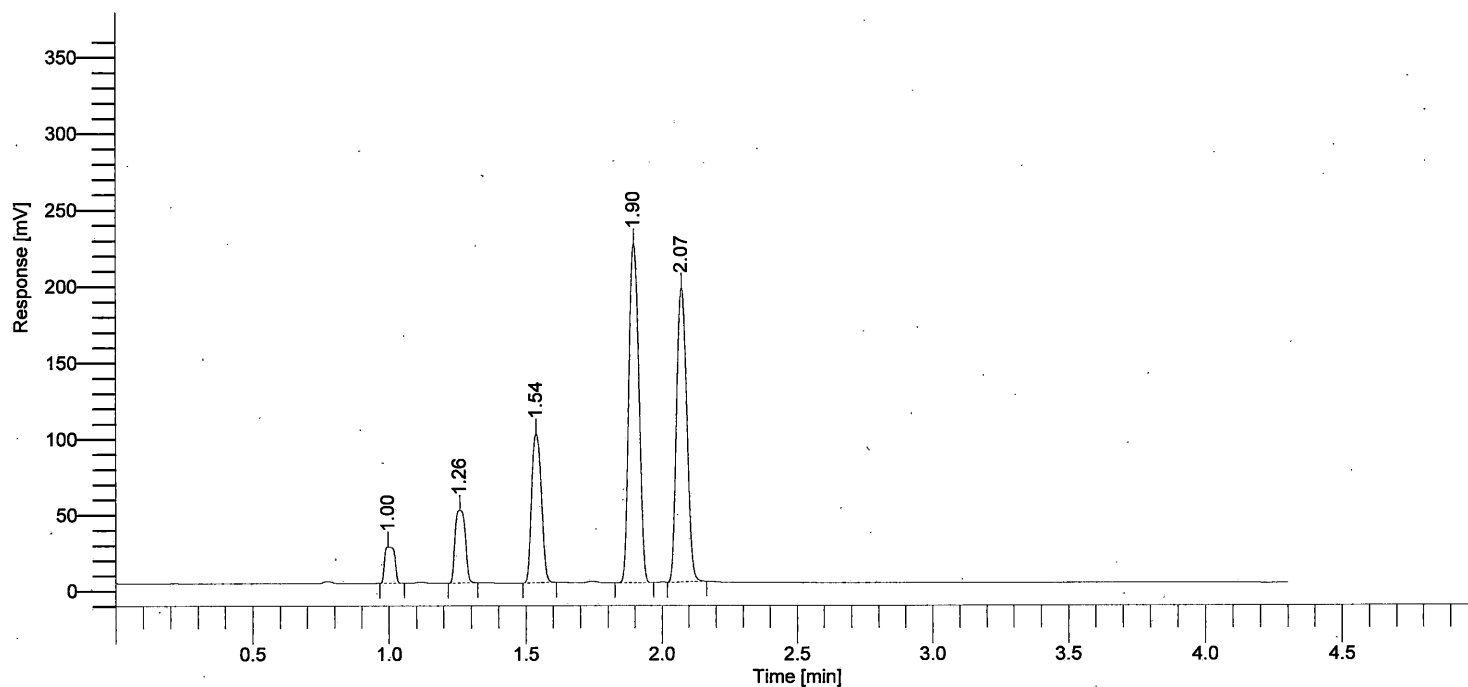

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [μV·s]
METHANOL	0.0798	1.00	61996.6
ETHANOL	0.0780	1.26	120424.1
ISOPROPANOL	0.0791	1.54	246764.8
ACETONE	0.0807	1.90	568974.4
N-PROPANOL	-----	2.07	516387.6

4 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36835
Sample Name : COMPOSITE
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 1

Date : 12/19/2017 9:10:39 AM
Data Acquisition Time : 12/19/2017 9:06:12 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-001.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

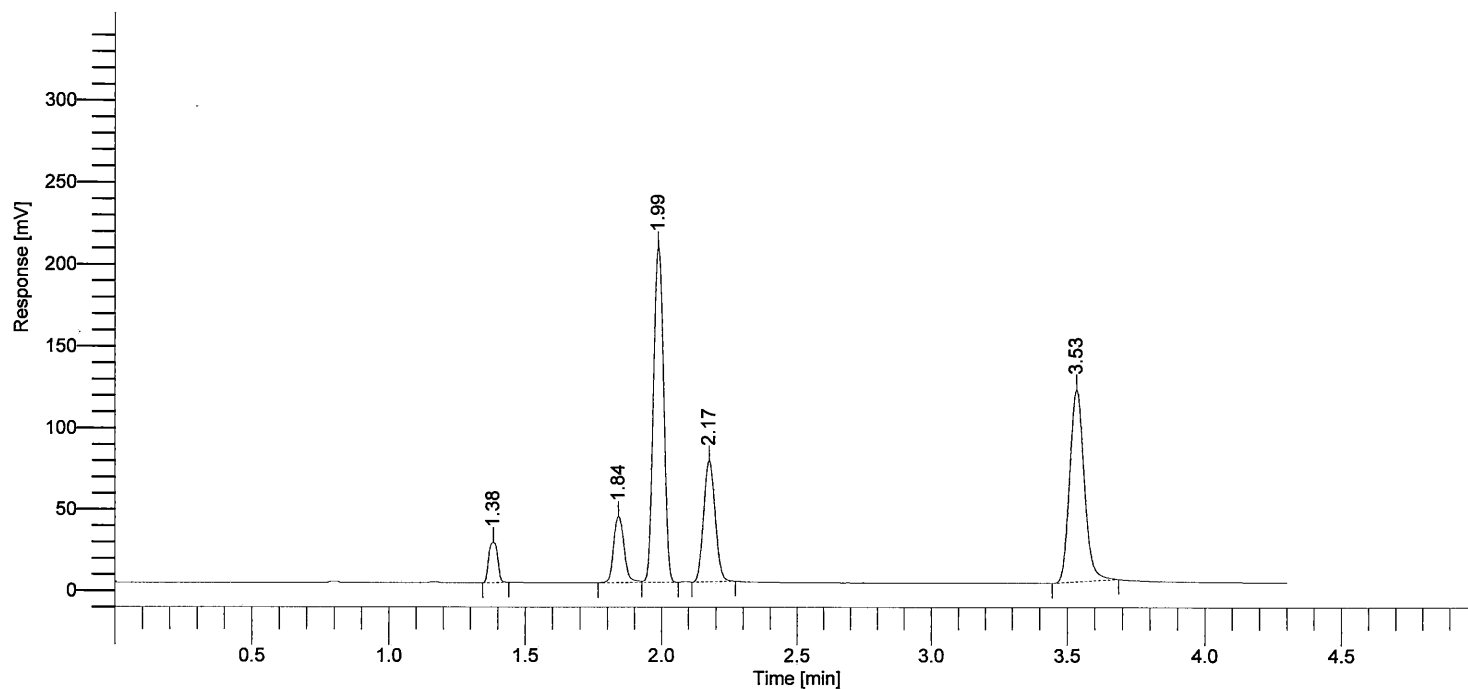

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
METHANOL	1.38
ETHANOL	1.84
ACETONE	1.99
ISOPROPANOL	2.17
N-PROPANOL	3.53

5 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36836
Sample Name : 0.08% CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 2

Date : 12/19/2017 9:15:37 AM
Data Acquisition Time : 12/19/2017 9:11:12 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-002.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

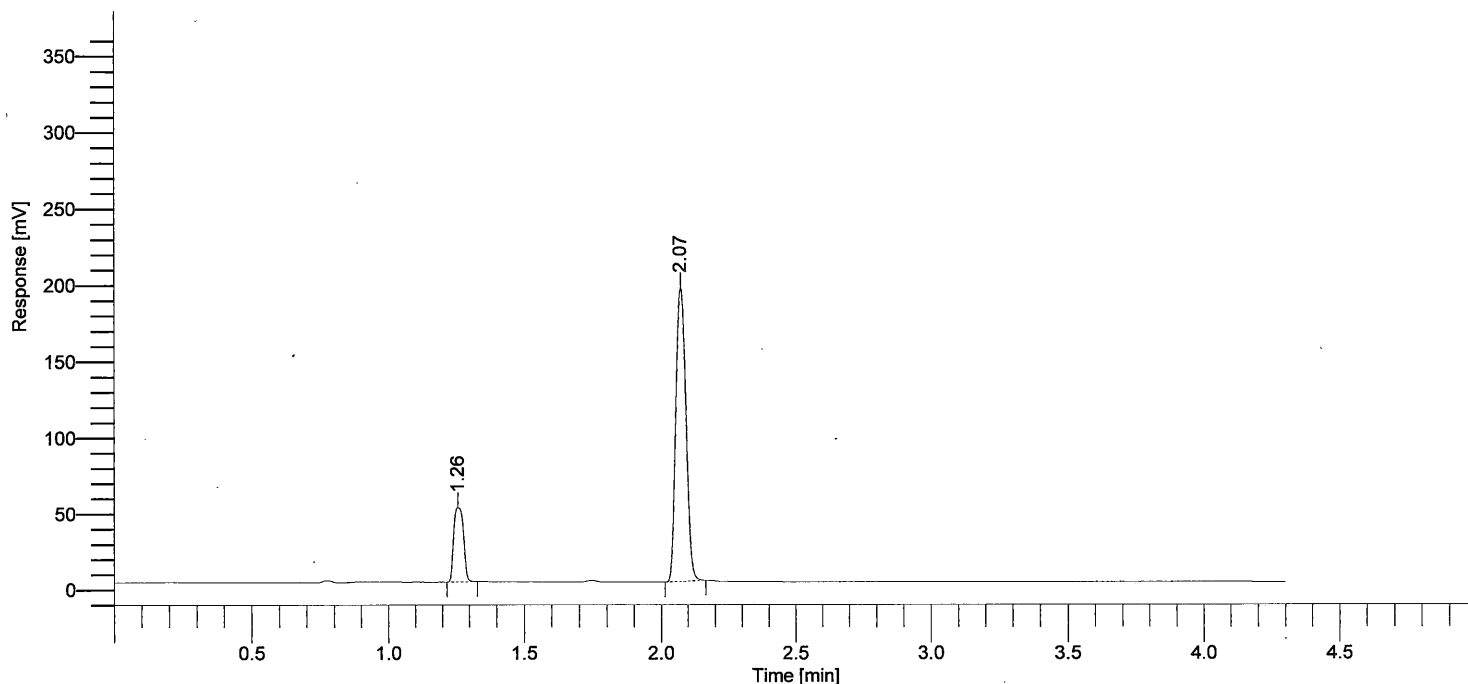

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"

Component Name	% by Wt	Time [min]	Area [μ V·s]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.0790	1.26	122118.8
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	516415.5


6 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36837
Sample Name : 0.08% CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 2

Date : 12/19/2017 9:15:39 AM

Data Acquisition Time : 12/19/2017 9:11:12 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-002.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

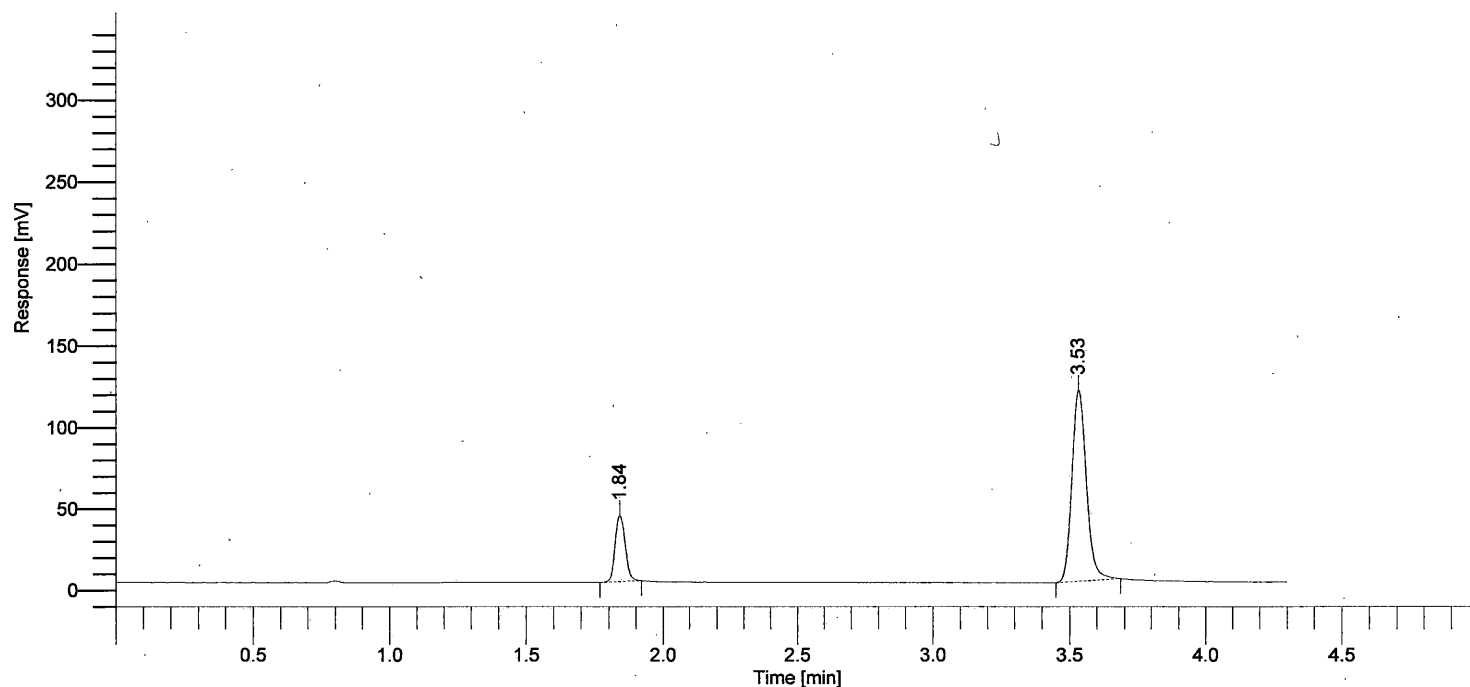

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

7 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36838
Sample Name : 0.10% CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 3

Date : 12/19/2017 9:20:37 AM
Data Acquisition Time : 12/19/2017 9:16:12 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-003.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

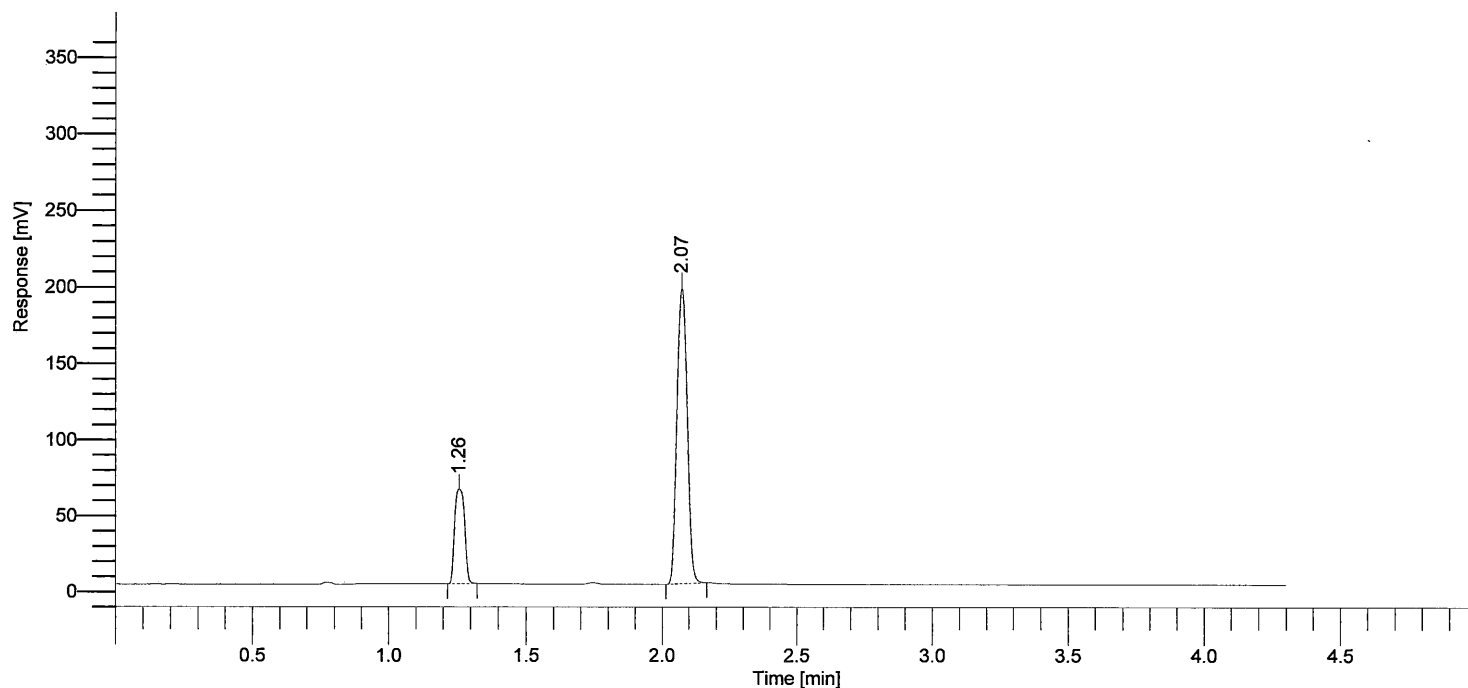

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.0984	1.26	154501.7
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	522243.8

8 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36839
Sample Name : 0.10% CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 3

Date : 12/19/2017 9:20:39 AM
Data Acquisition Time : 12/19/2017 9:16:12 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-003.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

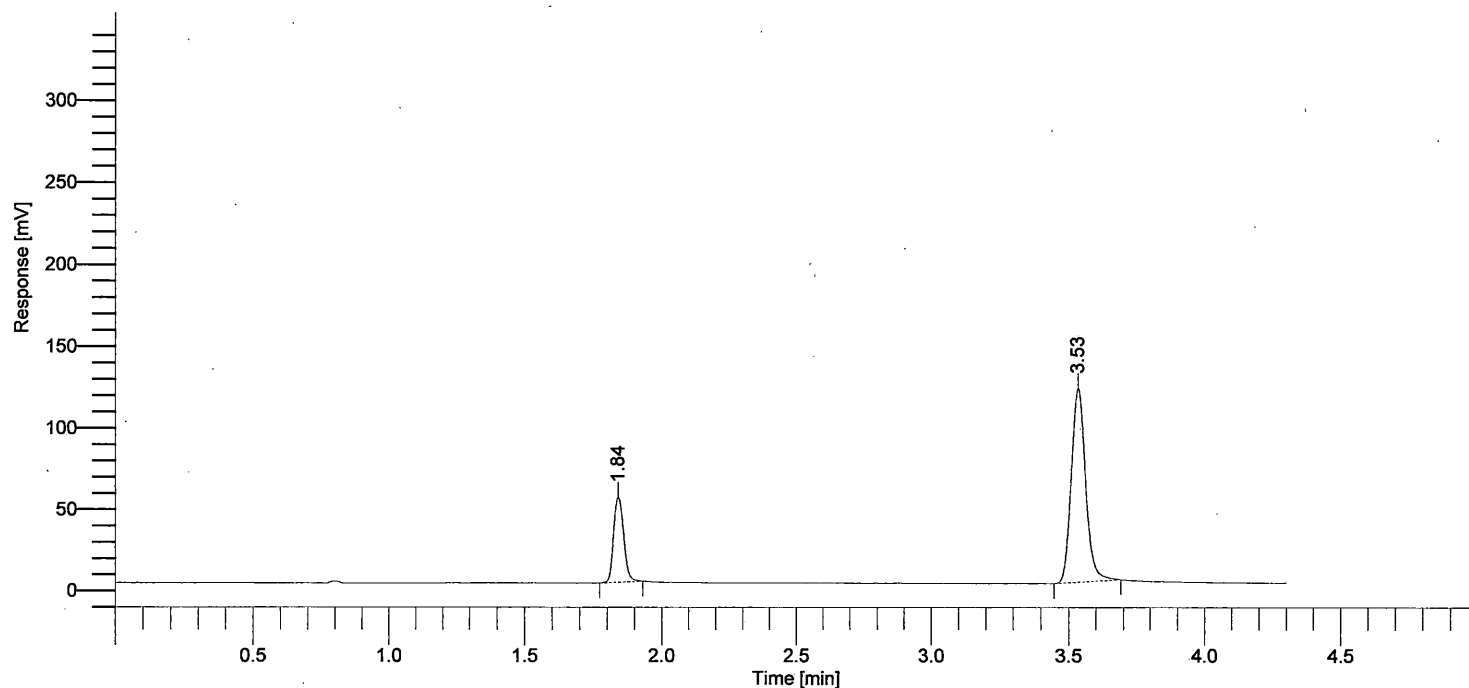

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

96

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36840
Sample Name : NEG CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 4

Date : 12/19/2017 9:25:37 AM
Data Acquisition Time : 12/19/2017 9:21:12 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-004.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

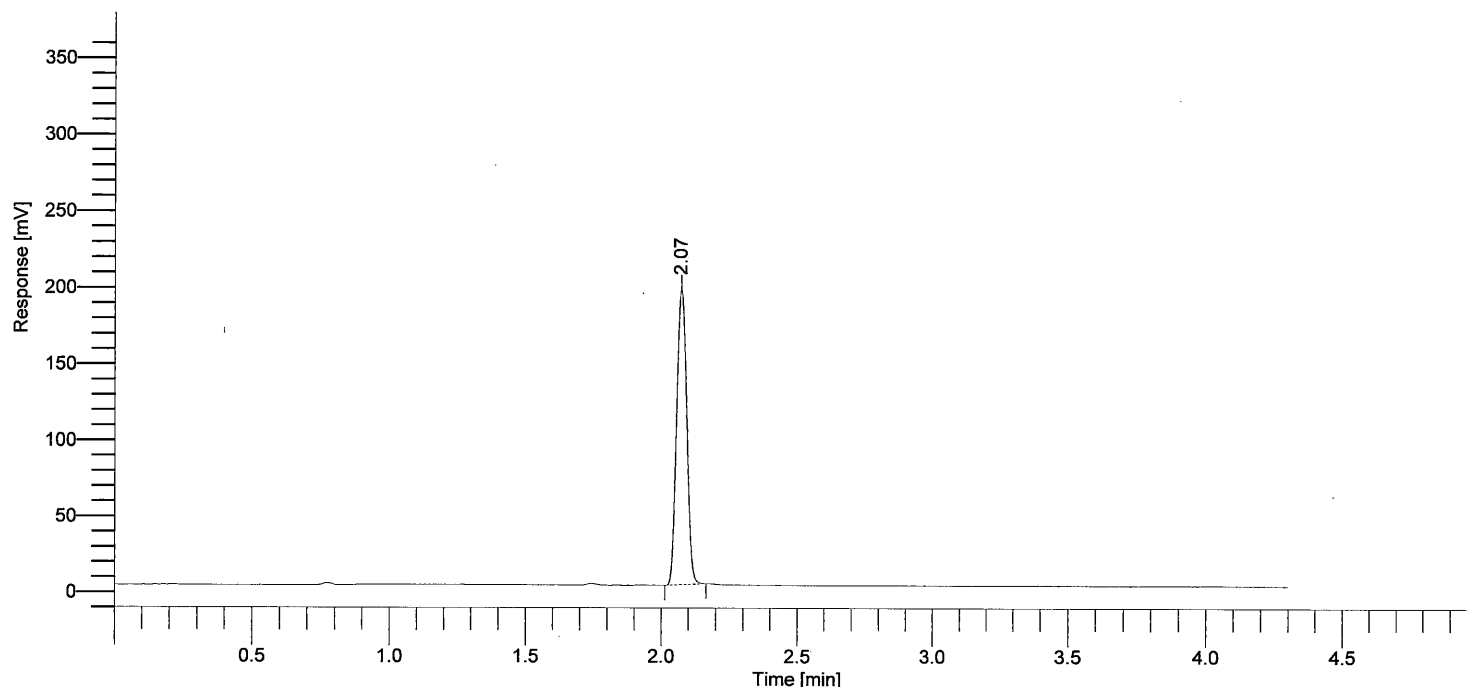

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.0000	1.26	0.0
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	518357.8

10 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36841
Sample Name : NEG CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 4

Date : 12/19/2017 9:25:39 AM
Data Acquisition Time : 12/19/2017 9:21:12 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-004.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

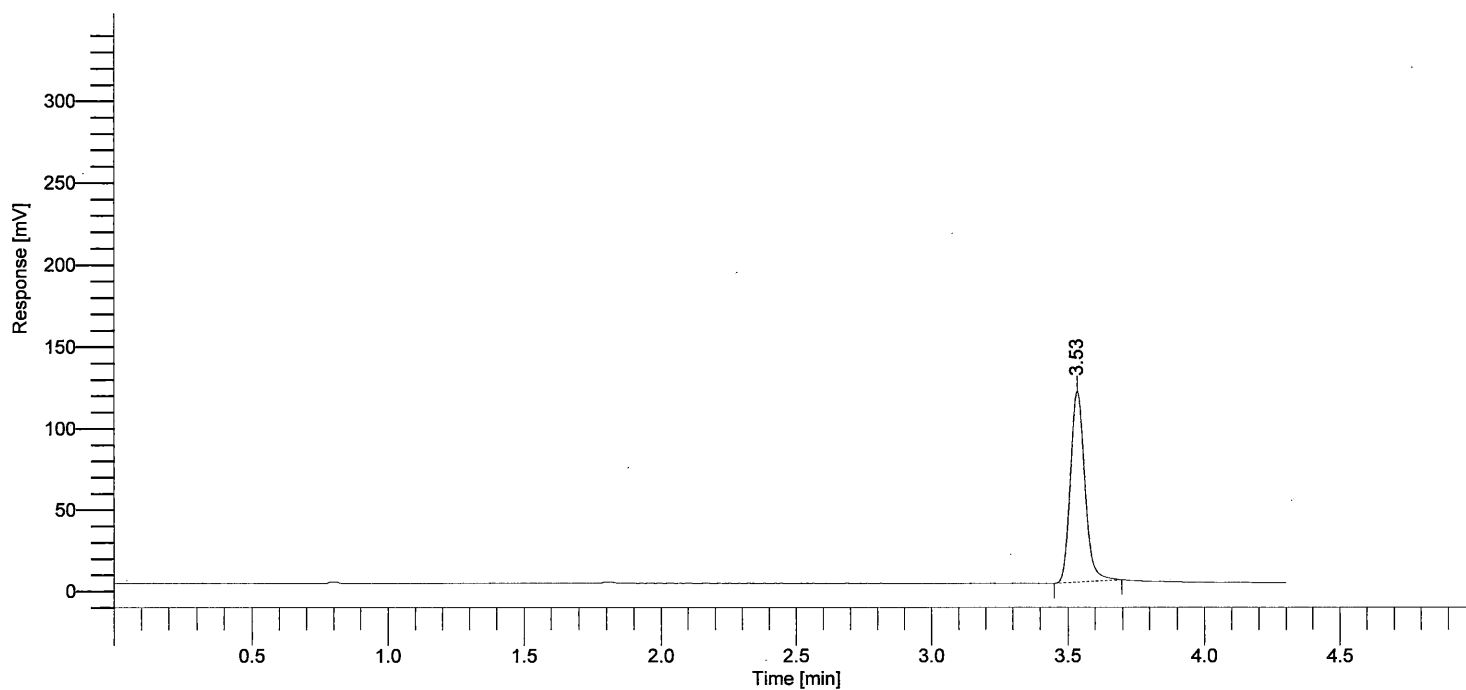

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
N-PROPANOL	3.53

11 am

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36842
Sample Name : GUTH 17390 #6
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 5

Date : 12/19/2017 9:30:37 AM
Data Acquisition Time : 12/19/2017 9:26:12 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-005.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

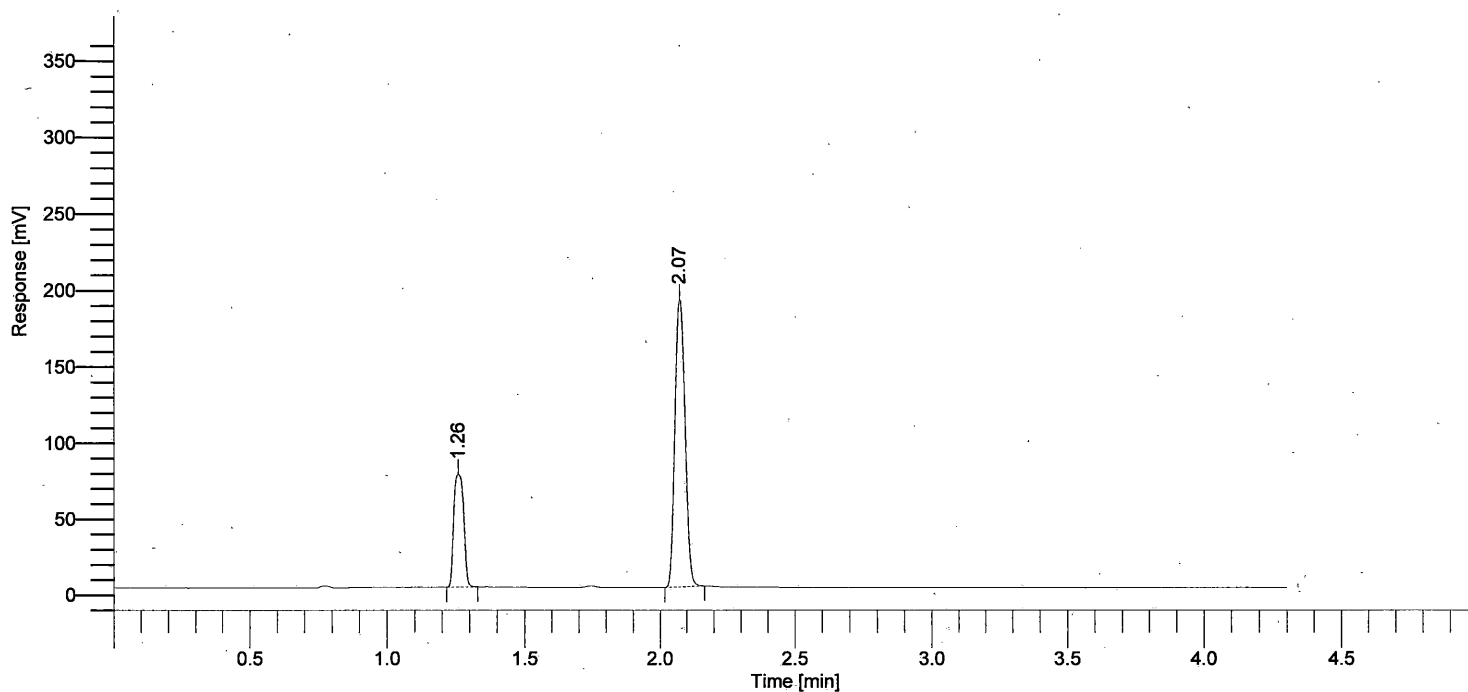

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.1207	1.26	184711.0
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	507278.1

12 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36843
Sample Name : GUTH 17390 #6
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 5

Date : 12/19/2017 9:30:39 AM
Data Acquisition Time : 12/19/2017 9:26:12 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-005.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

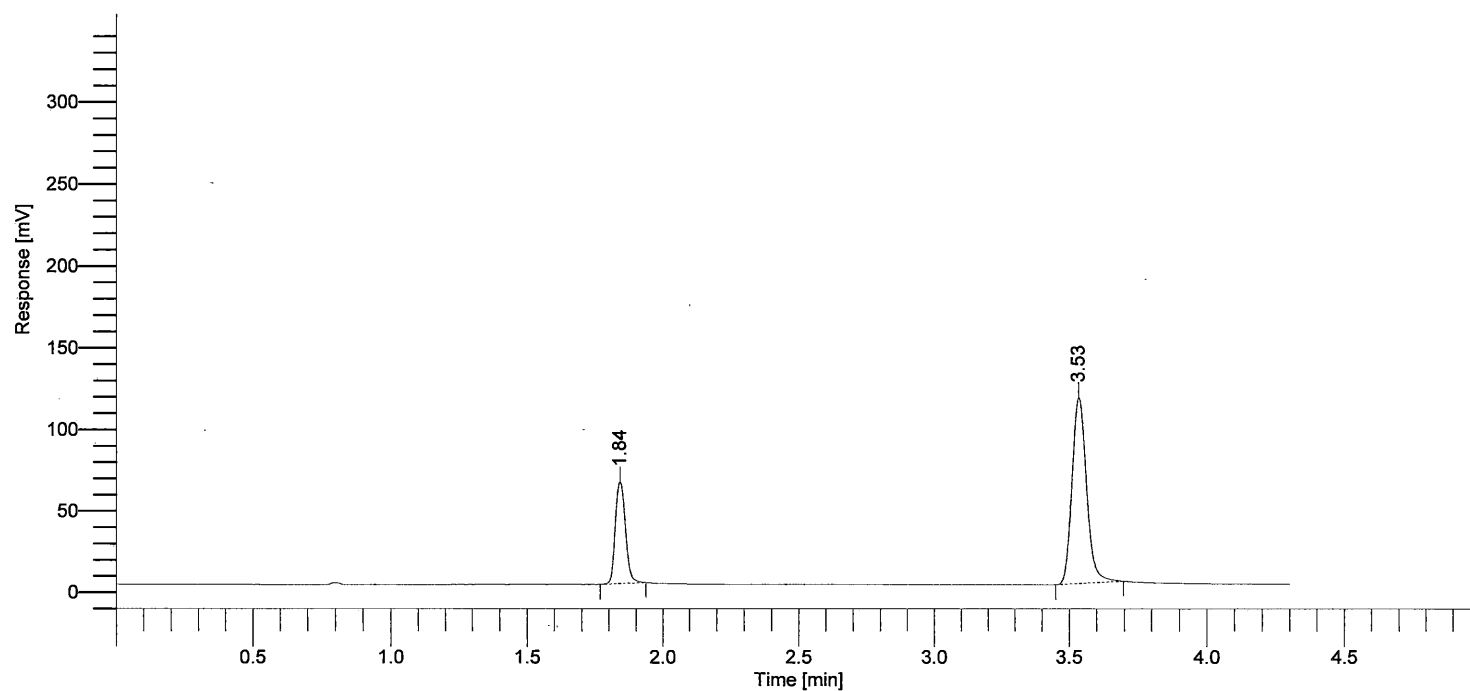

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

13 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36844
Sample Name : GUTH 17390 #6
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 6

Date : 12/19/2017 9:35:38 AM
Data Acquisition Time : 12/19/2017 9:31:12 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-006.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

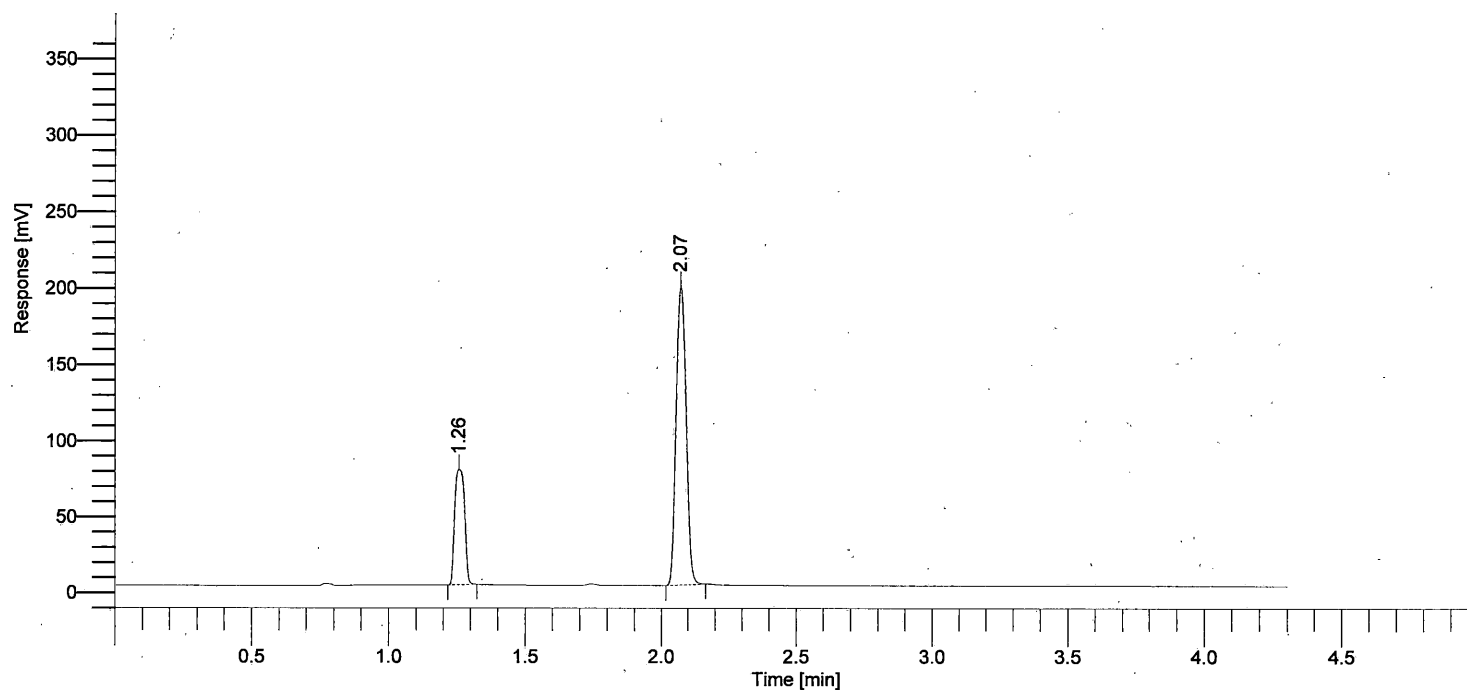

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [μ V·s]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.1196	1.26	188516.8
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	522745.5

14 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36845
Sample Name : GUTH 17390 #6
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 6

Date : 12/19/2017 9:35:39 AM
Data Acquisition Time : 12/19/2017 9:31:12 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-006.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

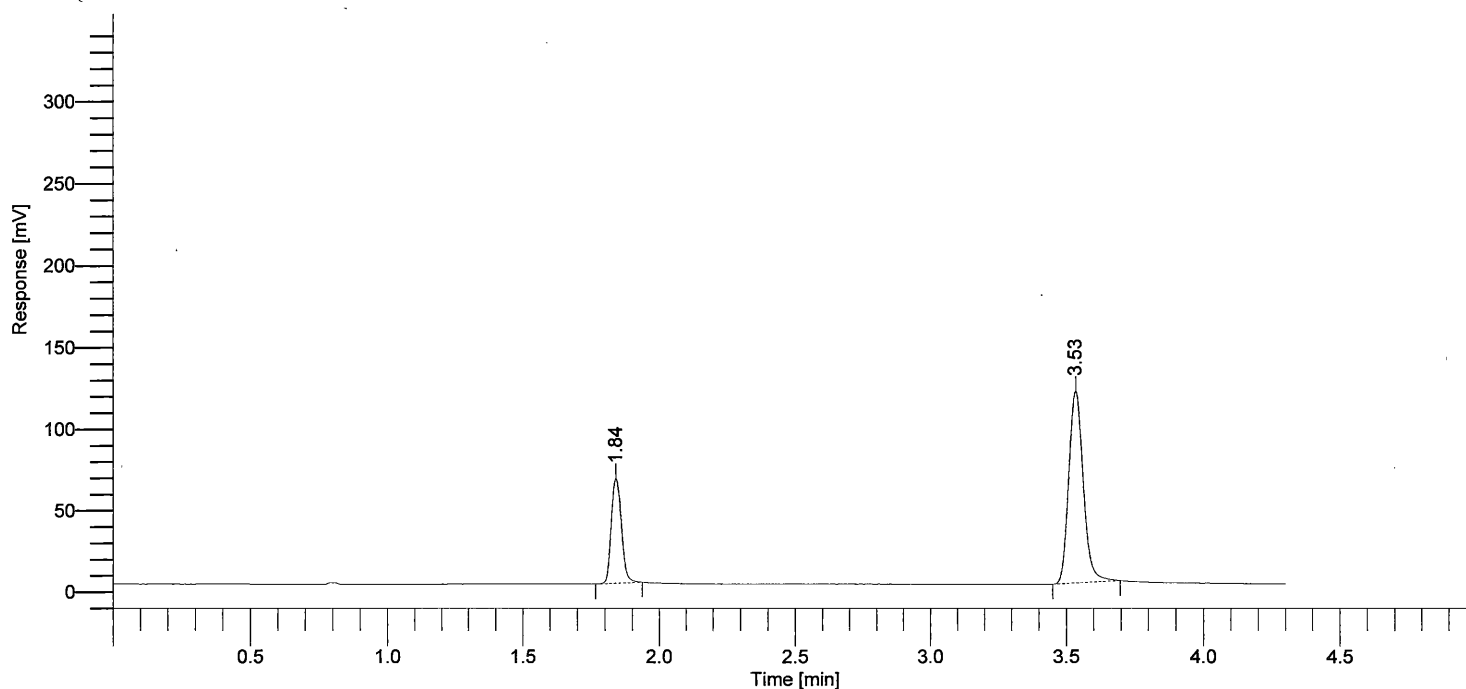

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

15 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36846
Sample Name : GUTH 17390 #6
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 7

Date : 12/19/2017 9:40:37 AM
Data Acquisition Time : 12/19/2017 9:36:12 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-007.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

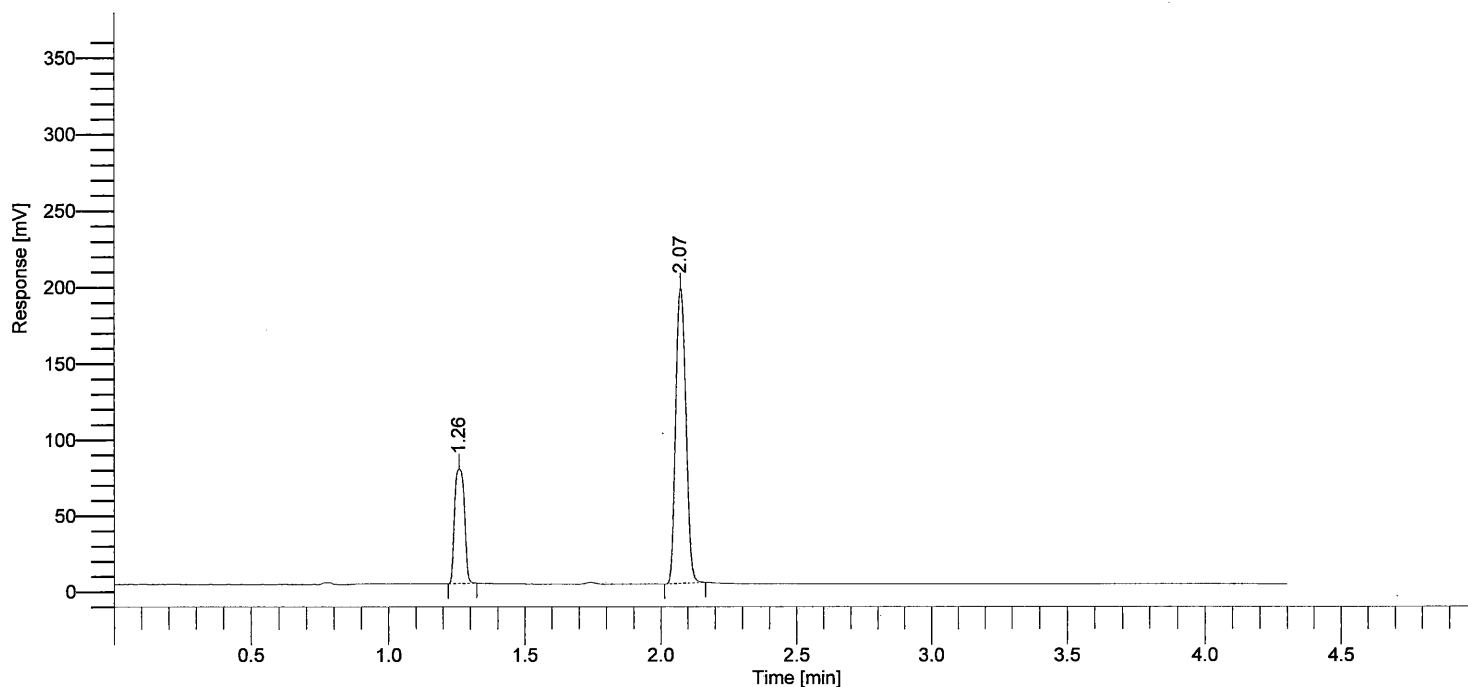

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [μ V-s]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.1198	1.26	187918.9
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	520038.4

He Cam

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36847
Sample Name : GUTH 17390 #6
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 7

Date : 12/19/2017 9:40:39 AM
Data Acquisition Time : 12/19/2017 9:36:12 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-007.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

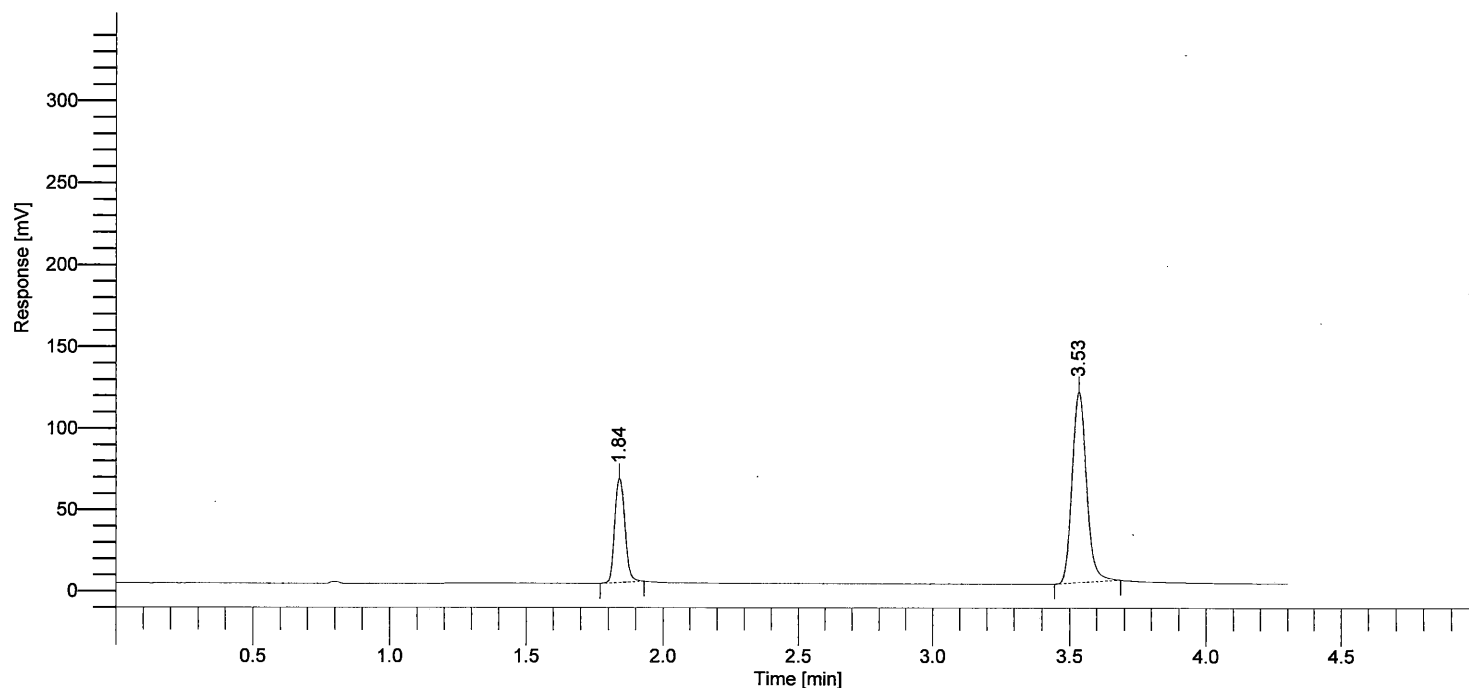

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

17 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36848
Sample Name : GUTH 17390 #7
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 8

Date : 12/19/2017 9:45:37 AM
Data Acquisition Time : 12/19/2017 9:41:12 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-008.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

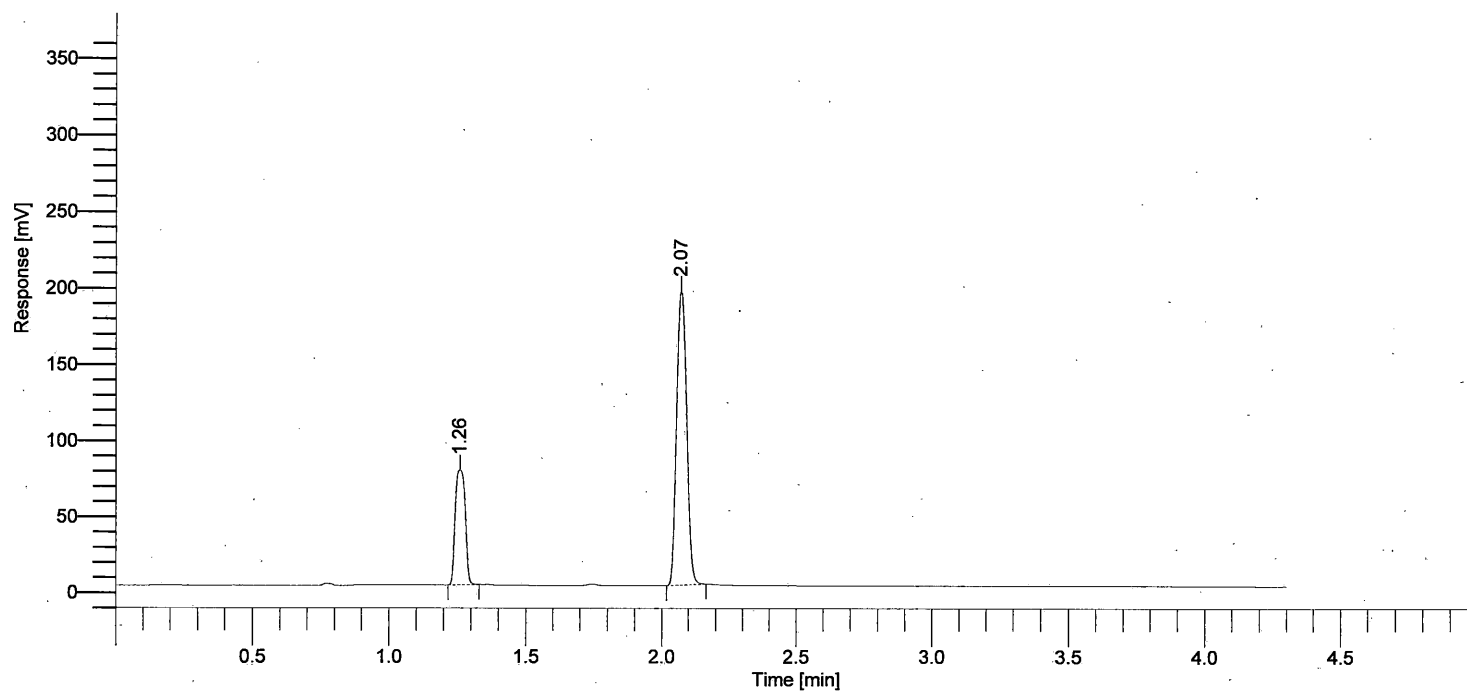

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [μ V·s]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.1202	1.26	188158.2
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	519011.1

18 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36849
Sample Name : GUTH 17390 #7
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 8

Date : 12/19/2017 9:45:39 AM
Data Acquisition Time : 12/19/2017 9:41:12 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-008.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

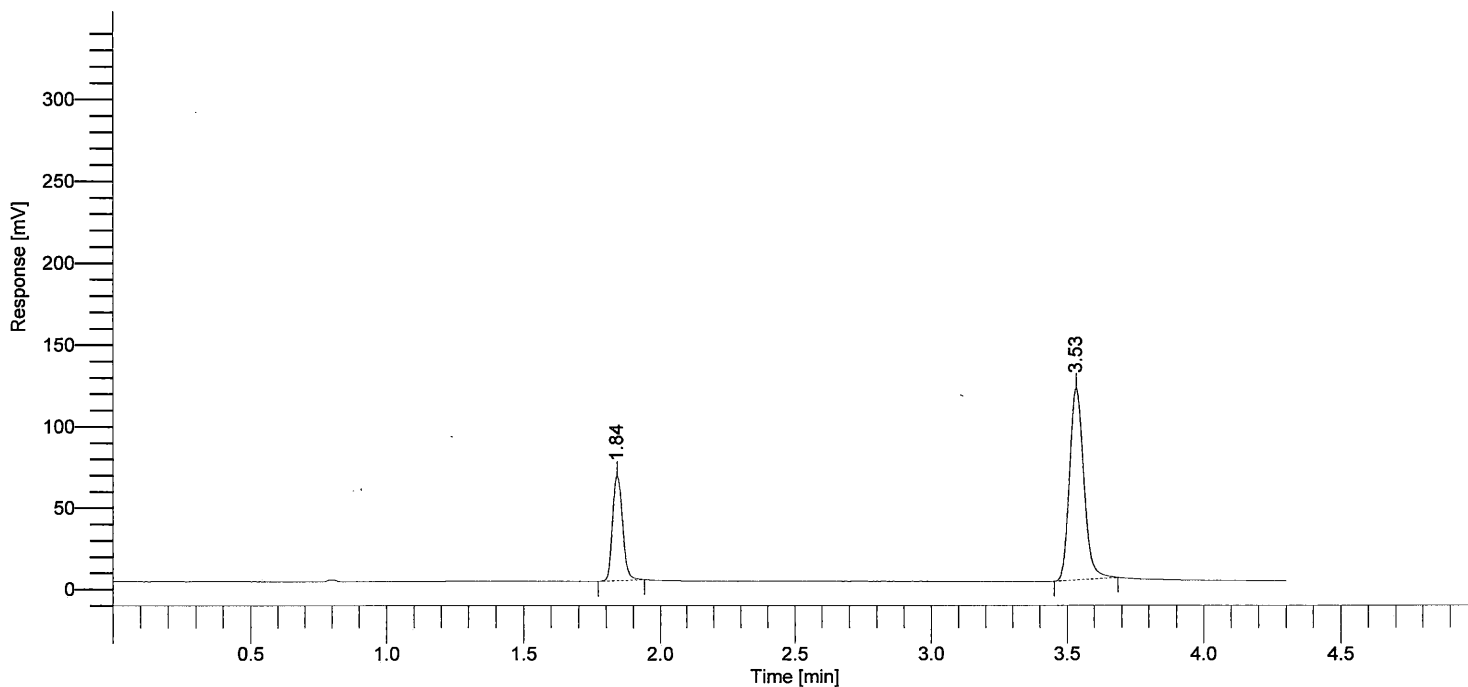

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

19 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36850
Sample Name : GUTH 17390 #7
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 9

Date : 12/19/2017 9:50:38 AM
Data Acquisition Time : 12/19/2017 9:46:12 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-009.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

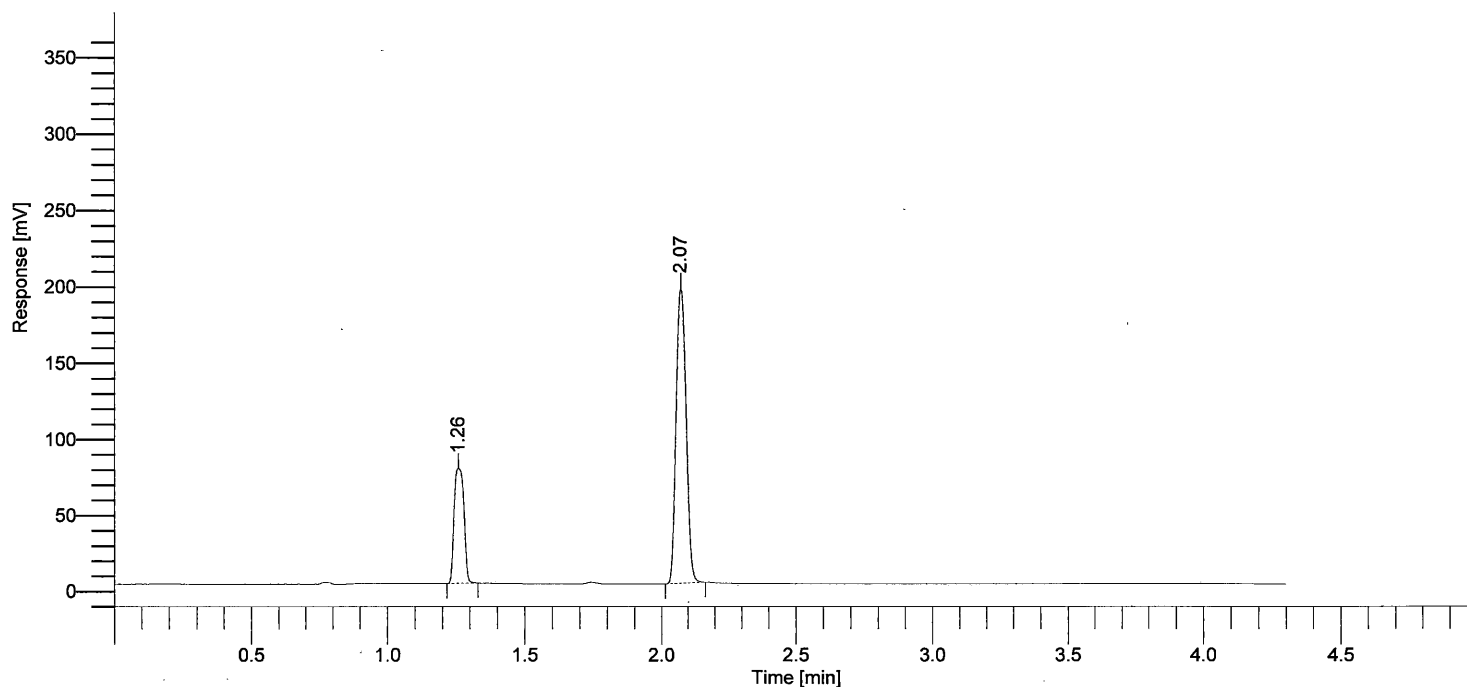

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.1203	1.26	188340.7
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	519075.0

20 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36851
Sample Name : GUTH 17390 #7
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 9

Date : 12/19/2017 9:50:39 AM
Data Acquisition Time : 12/19/2017 9:46:12 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-009.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

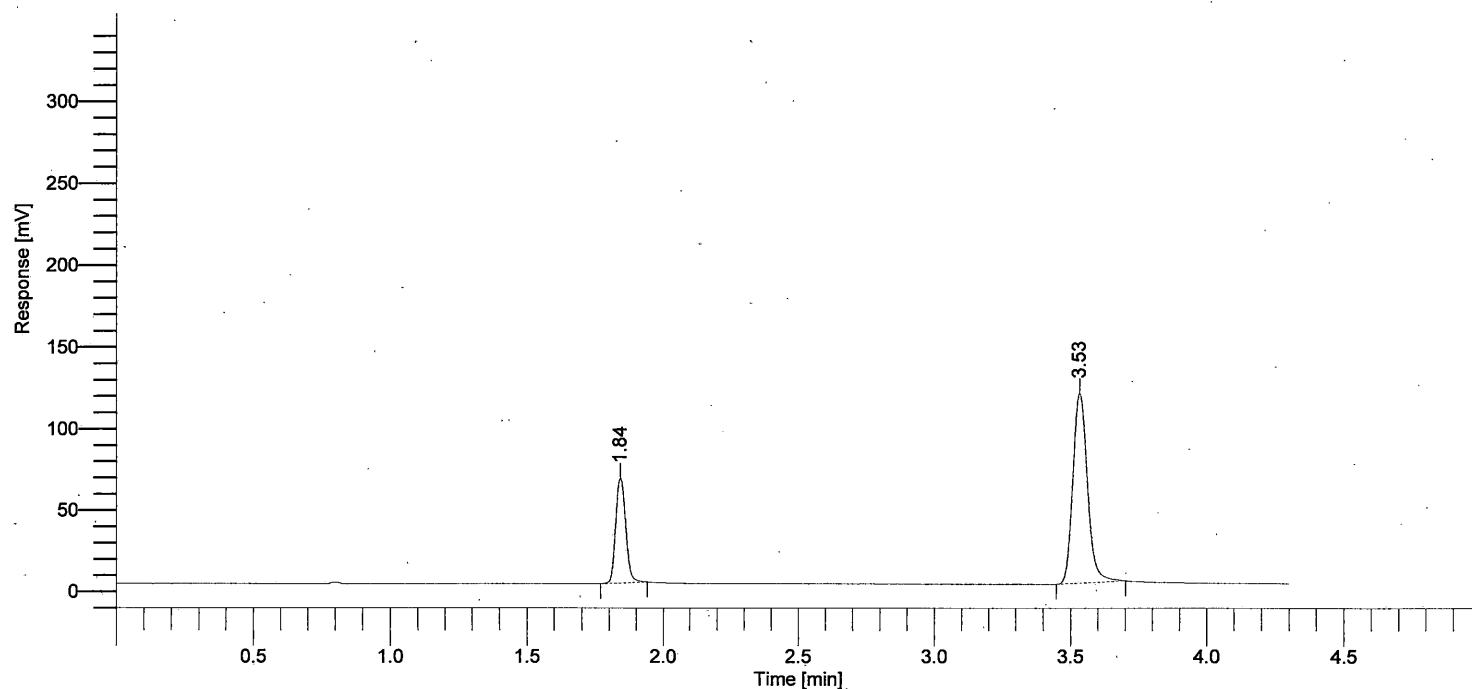

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

21 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36852
Sample Name : GUTH 17390 #7
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 10

Date : 12/19/2017 9:55:37 AM
Data Acquisition Time : 12/19/2017 9:51:12 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-010.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

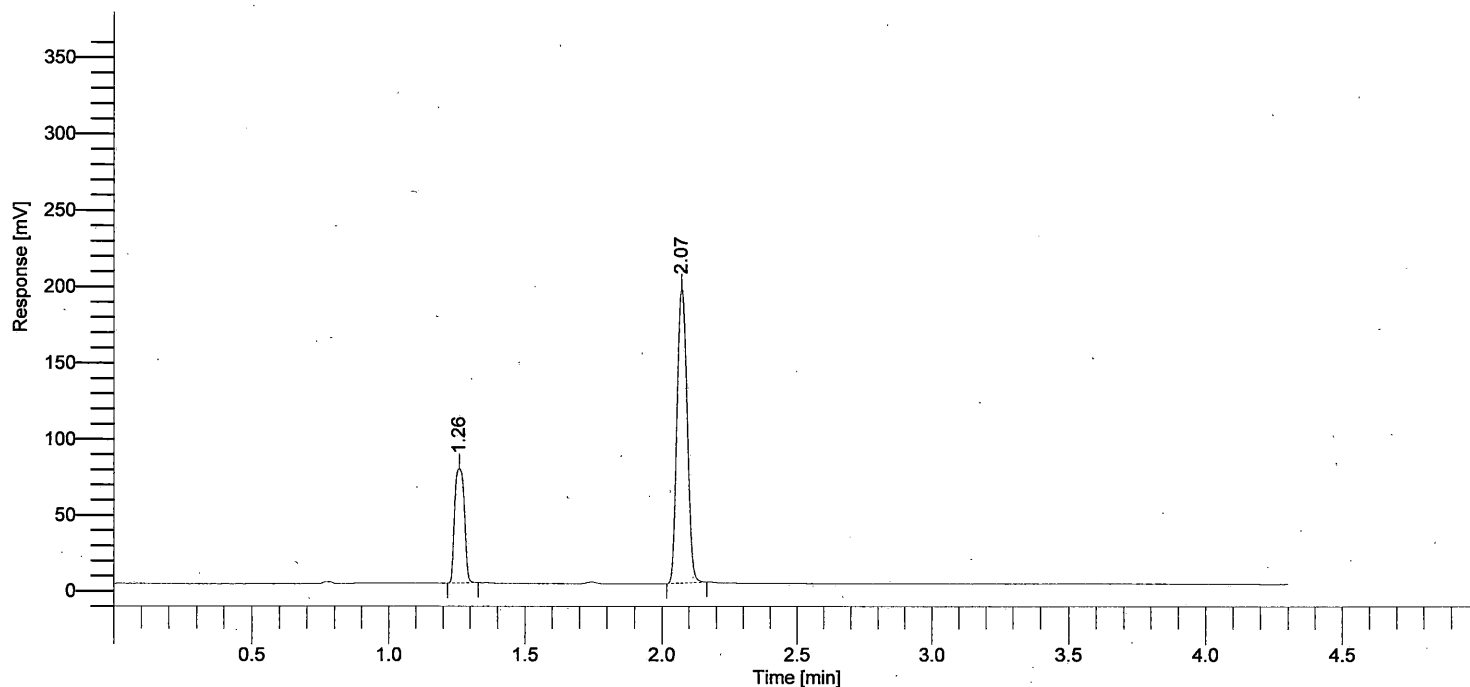

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [μ V·s]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.1201	1.26	187093.7
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	516648.0

22 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36853
Sample Name : GUTH 17390 #7
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 10

Date : 12/19/2017 9:55:39 AM
Data Acquisition Time : 12/19/2017 9:51:12 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-010.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

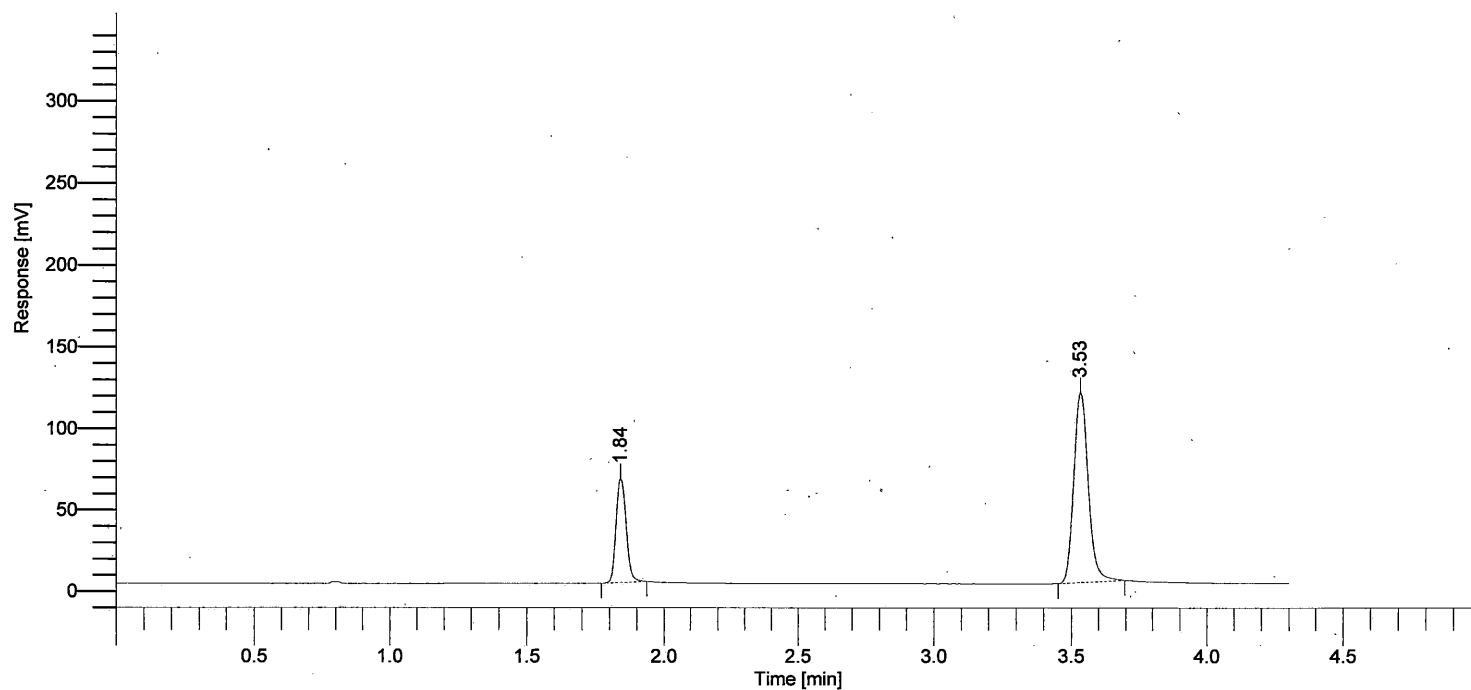

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

23 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36854
Sample Name : GUTH 17390 #707
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 11

Date : 12/19/2017 10:00:37 AM
Data Acquisition Time : 12/19/2017 9:56:12 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-011.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

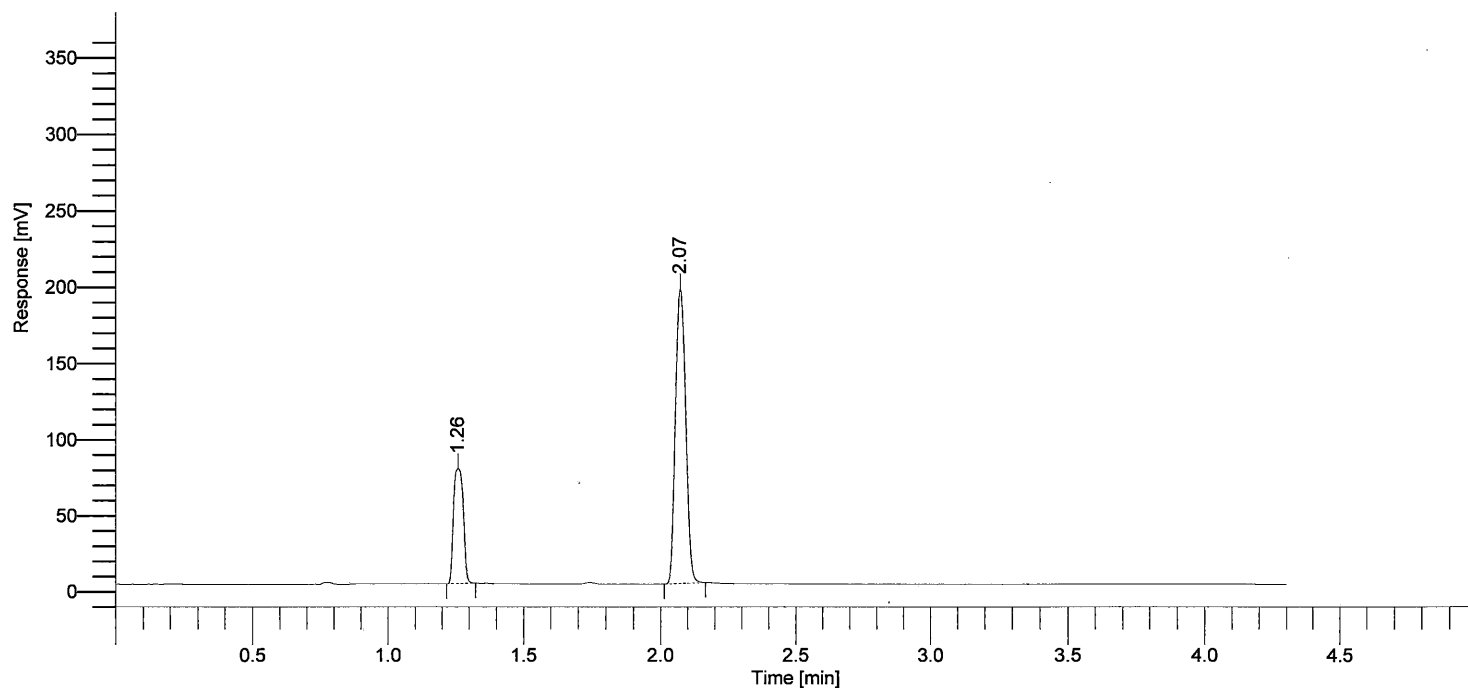

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.1204	1.26	187646.1
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	516840.4

24 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36855
Sample Name : GUTH 17390 #707
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 11

Date : 12/19/2017 10:00:39 AM
Data Acquisition Time : 12/19/2017 9:56:12 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-011.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

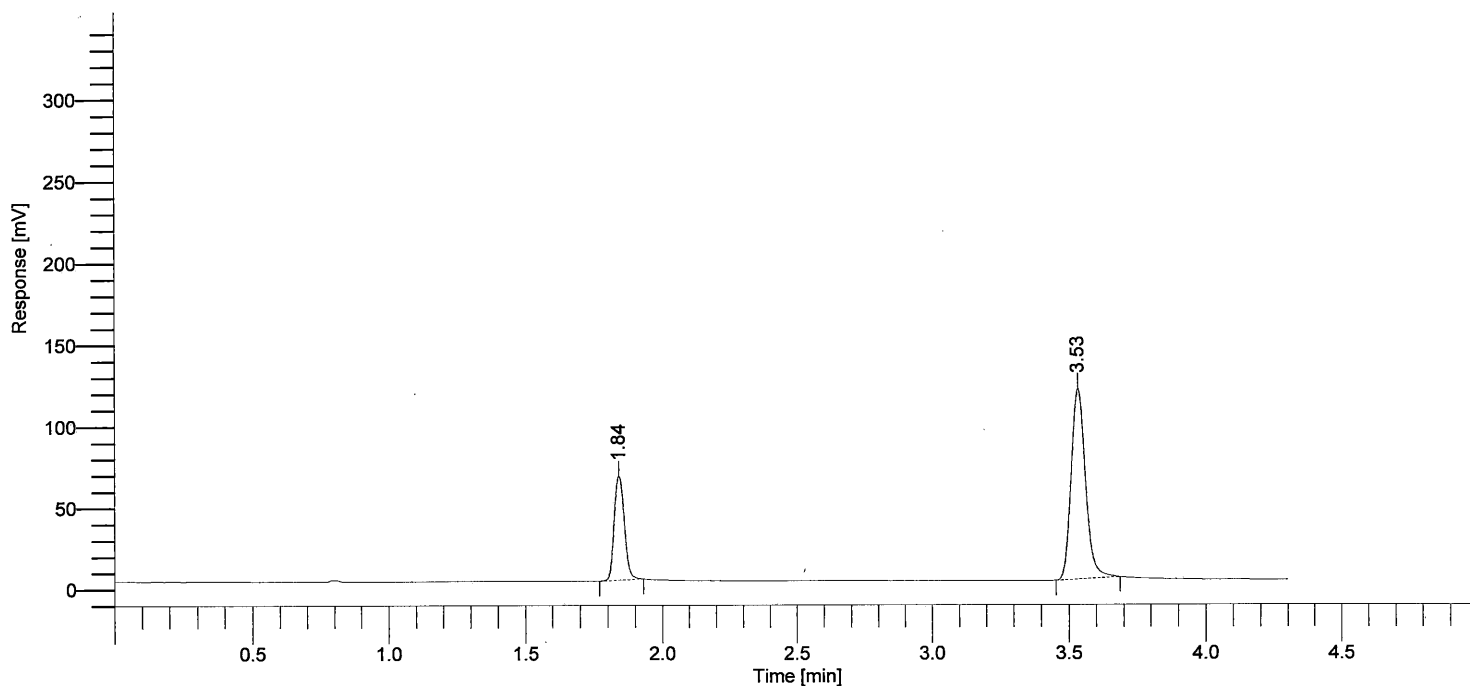

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

25 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36856
Sample Name : GUTH 17390 #707
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 12

Date : 12/19/2017 10:05:39 AM
Data Acquisition Time : 12/19/2017 10:01:12 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-012.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

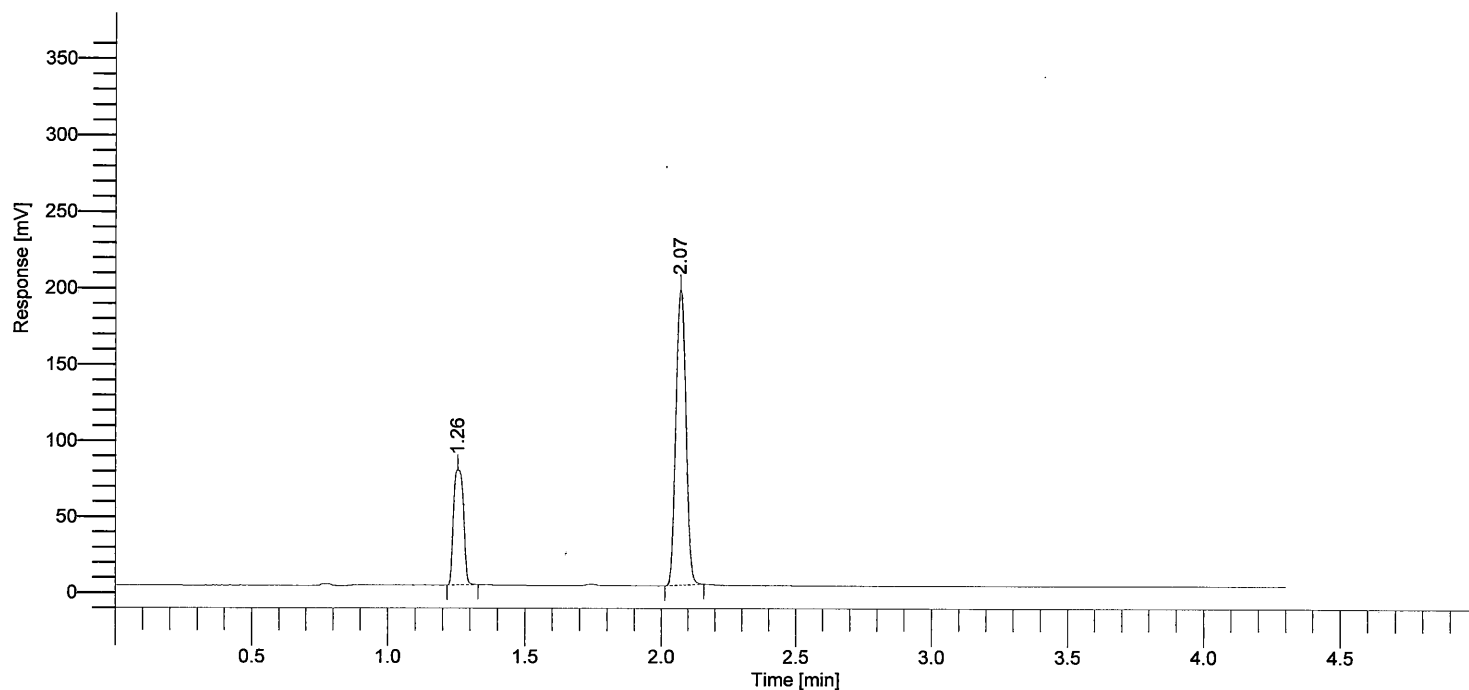

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.1205	1.26	189289.7
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	520752.4

26 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36857
Sample Name : GUTH 17390 #707
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 12

Date : 12/19/2017 10:05:40 AM
Data Acquisition Time : 12/19/2017 10:01:12 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-012.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

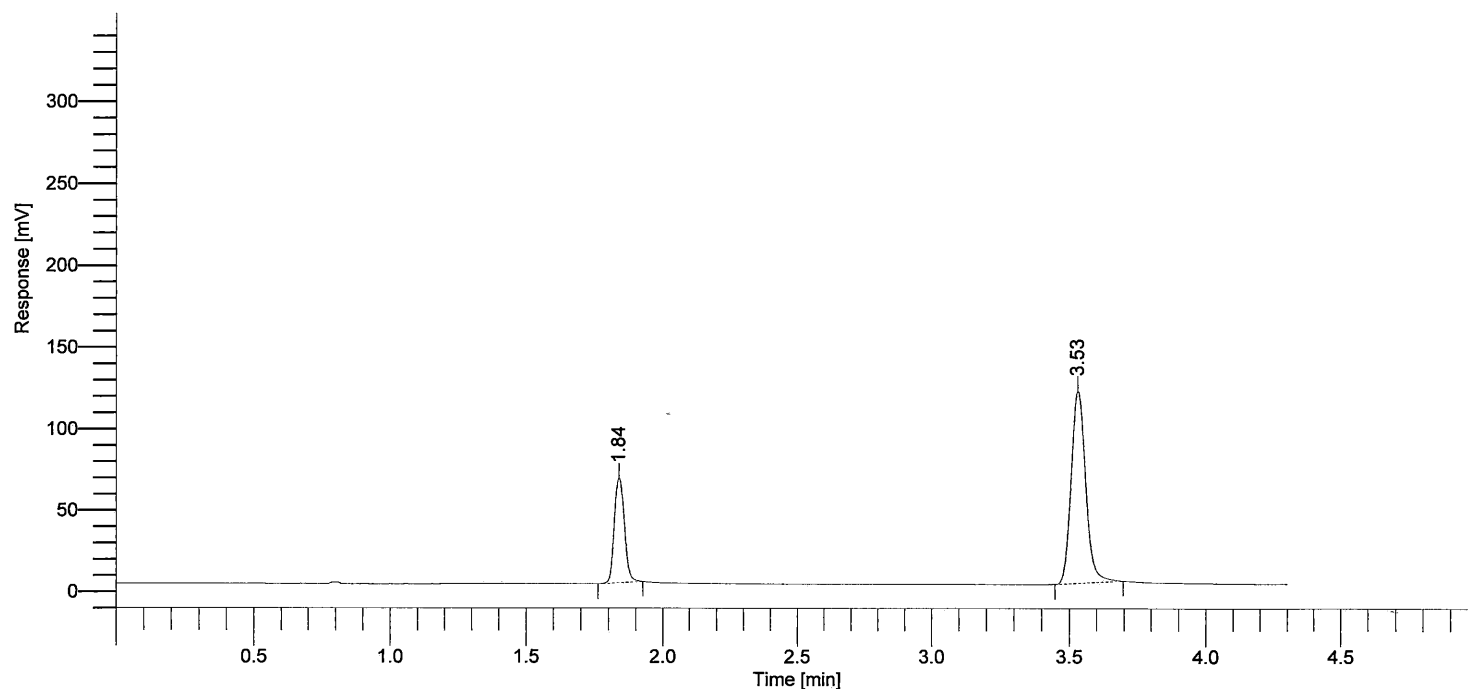

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

27 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36858
Sample Name : GUTH 17390 #707
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 13

Date : 12/19/2017 10:10:38 AM
Data Acquisition Time : 12/19/2017 10:06:12 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-013.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

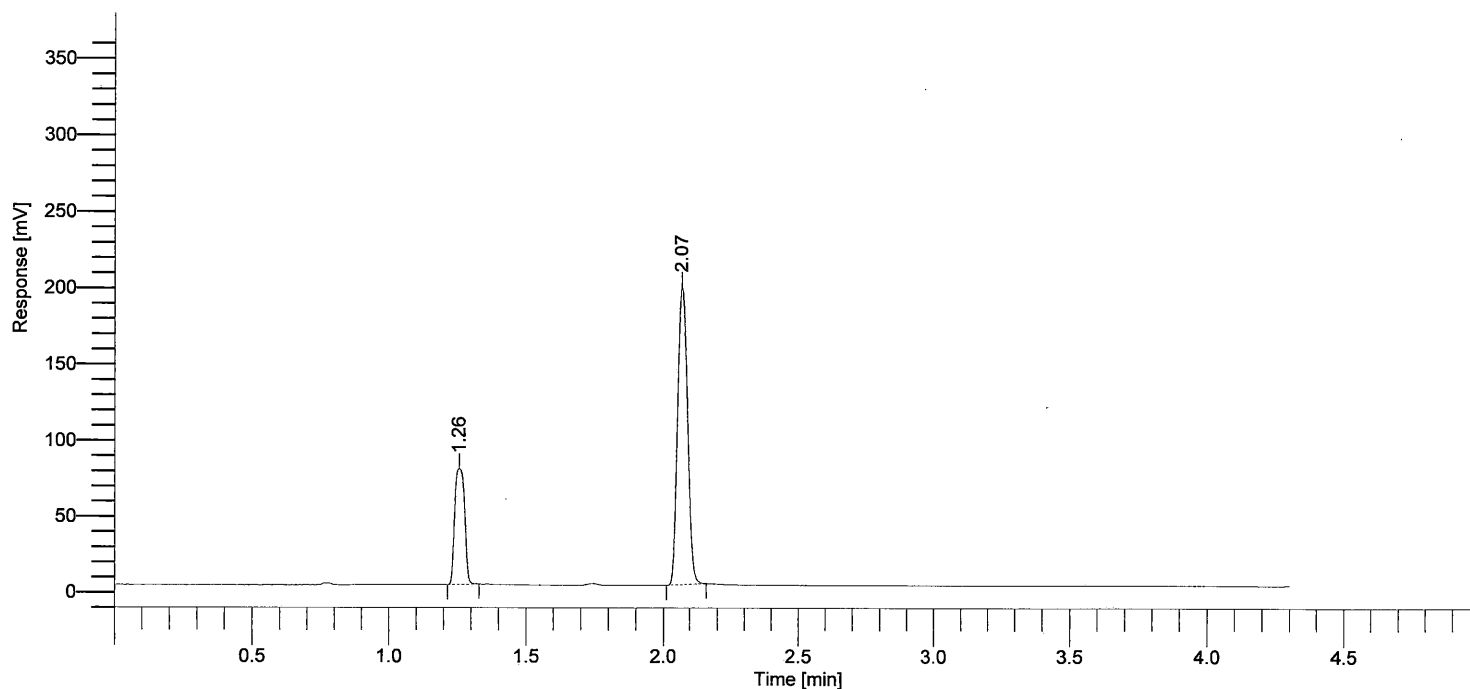

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [μ V·s]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.1205	1.26	189817.1
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	522187.9

28 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36859
Sample Name : GUTH 17390 #707
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 13

Date : 12/19/2017 10:10:39 AM
Data Acquisition Time : 12/19/2017 10:06:12 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-013.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

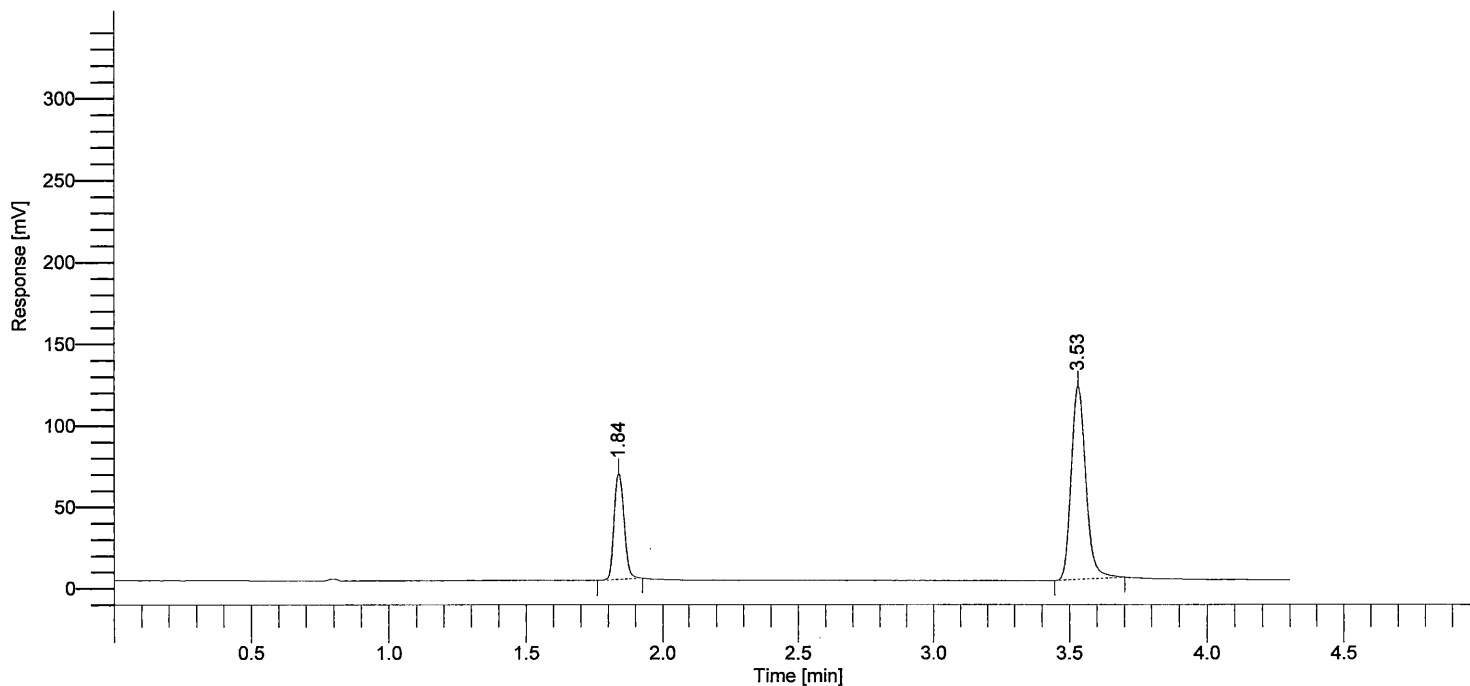

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

29 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36860
Sample Name : 0.10% CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 14

Date : 12/19/2017 10:15:38 AM
Data Acquisition Time : 12/19/2017 10:11:12 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-014.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

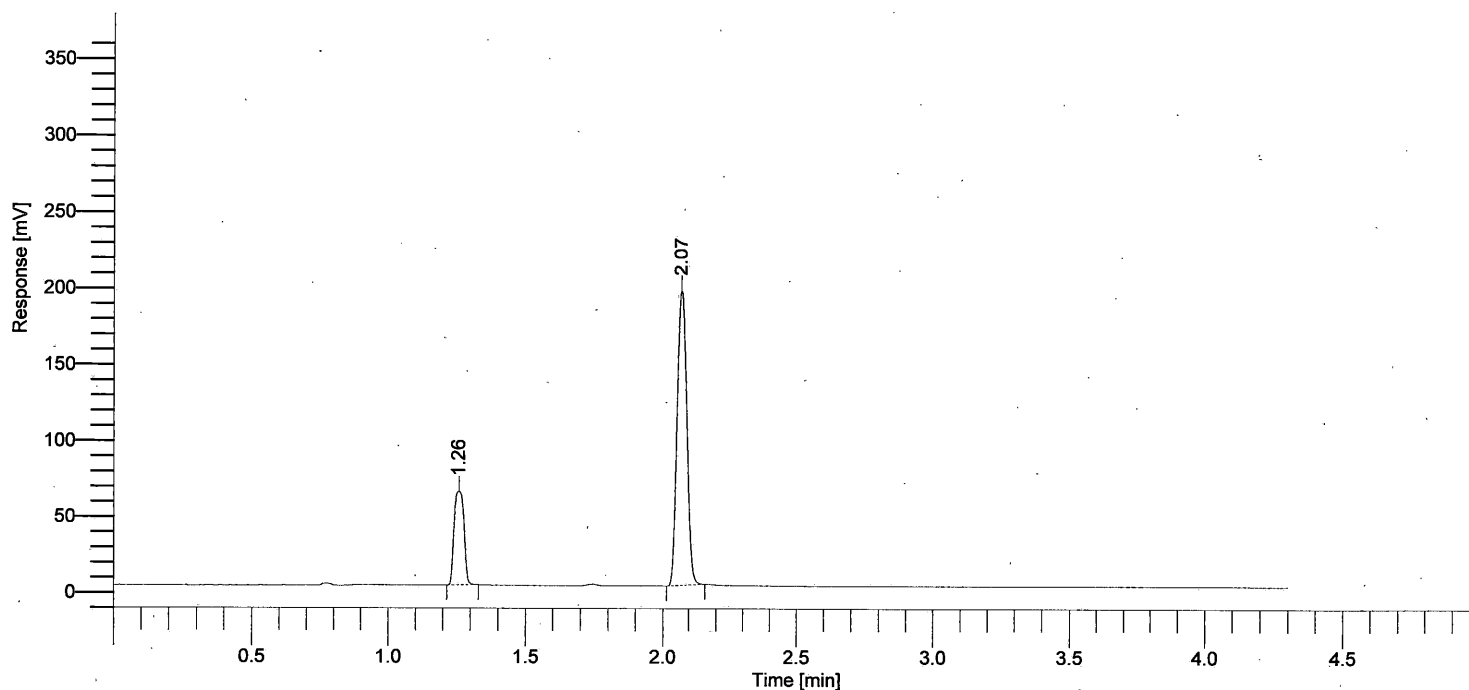

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [μ V·s]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.0988	1.26	153476.5
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	516916.5

30 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36861
Sample Name : 0.10% CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 14

Date : 12/19/2017 10:15:39 AM
Data Acquisition Time : 12/19/2017 10:11:12 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-014.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

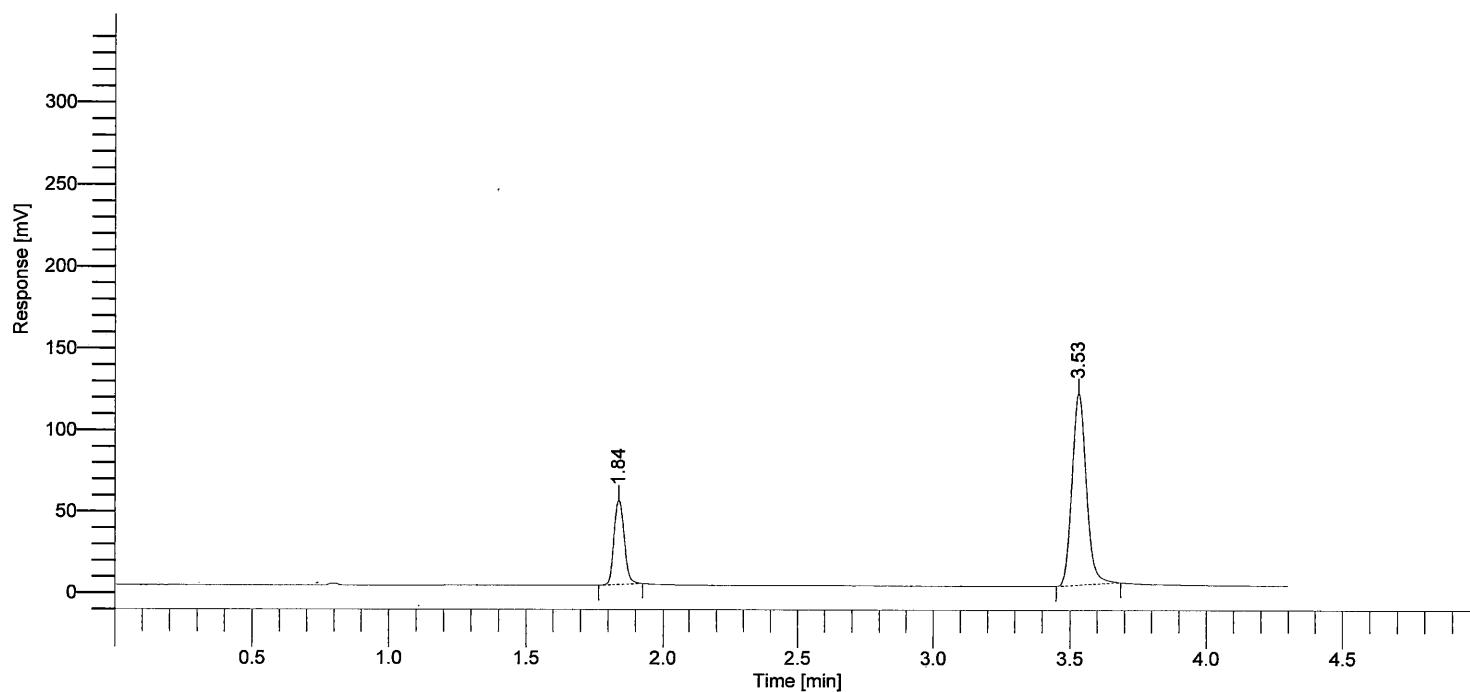

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

31 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36862
Sample Name : NEG CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 15

Date : 12/19/2017 10:20:38 AM
Data Acquisition Time : 12/19/2017 10:16:12 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-015.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

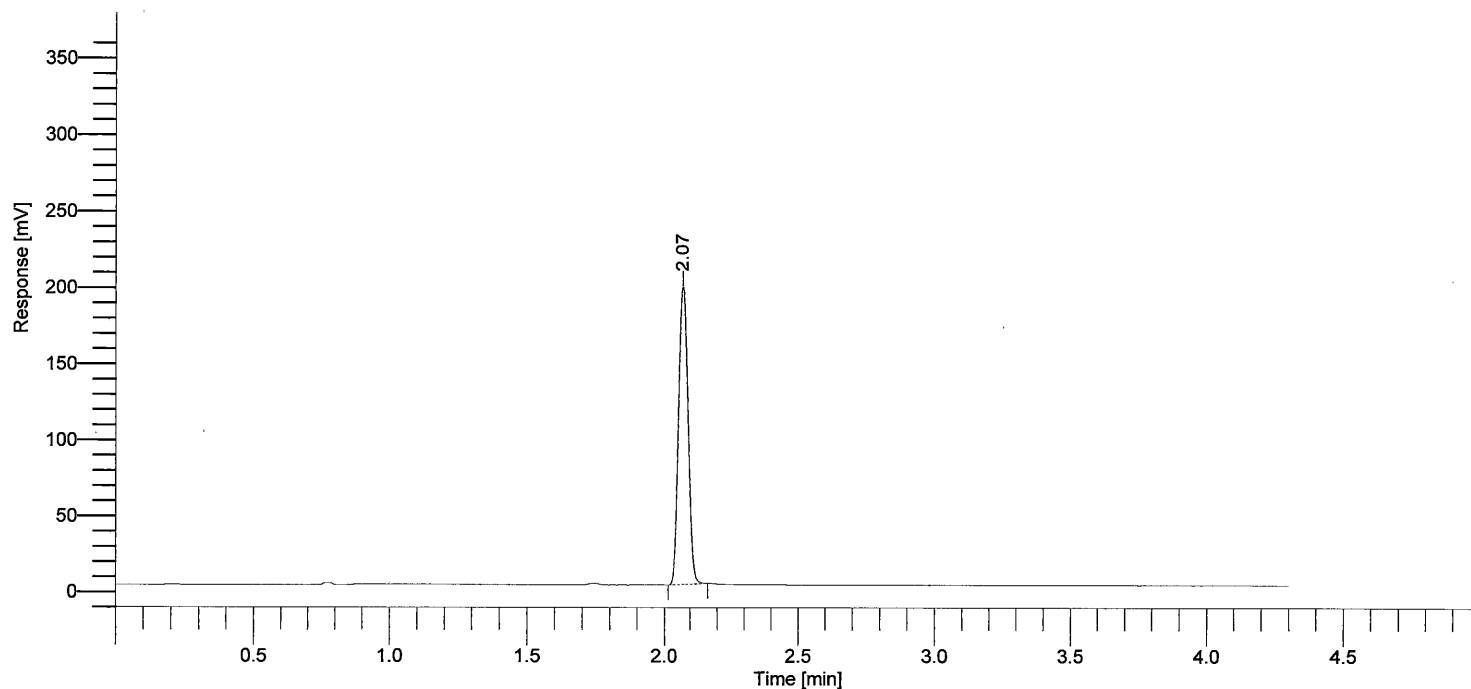

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [μ V·s]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.0000	1.26	0.0
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	522424.3

32 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36863
Sample Name : NEG CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 15

Date : 12/19/2017 10:20:39 AM
Data Acquisition Time : 12/19/2017 10:16:12 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-015.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

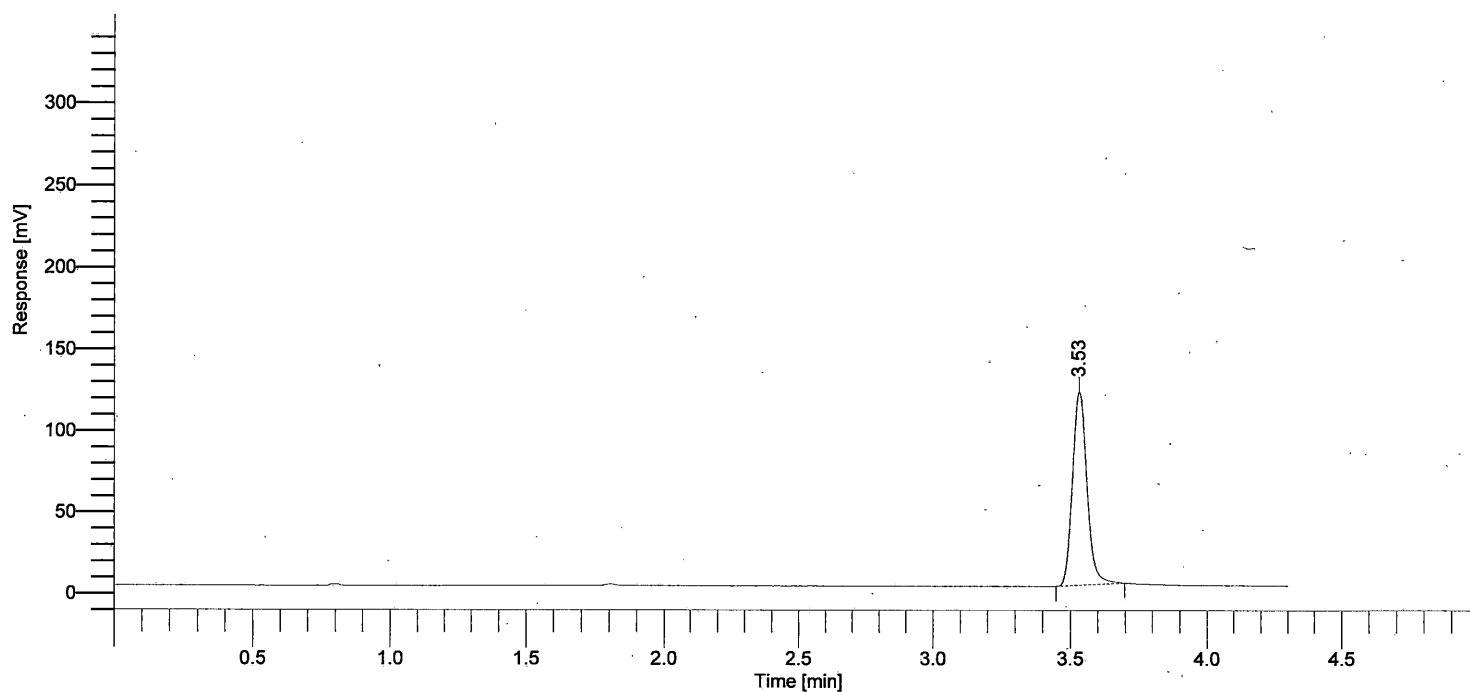

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
N-PROPANOL	3.53

33 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36864
Sample Name : GUTH 17390 #708
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 16

Date : 12/19/2017 10:25:38 AM
Data Acquisition Time : 12/19/2017 10:21:12 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-016.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

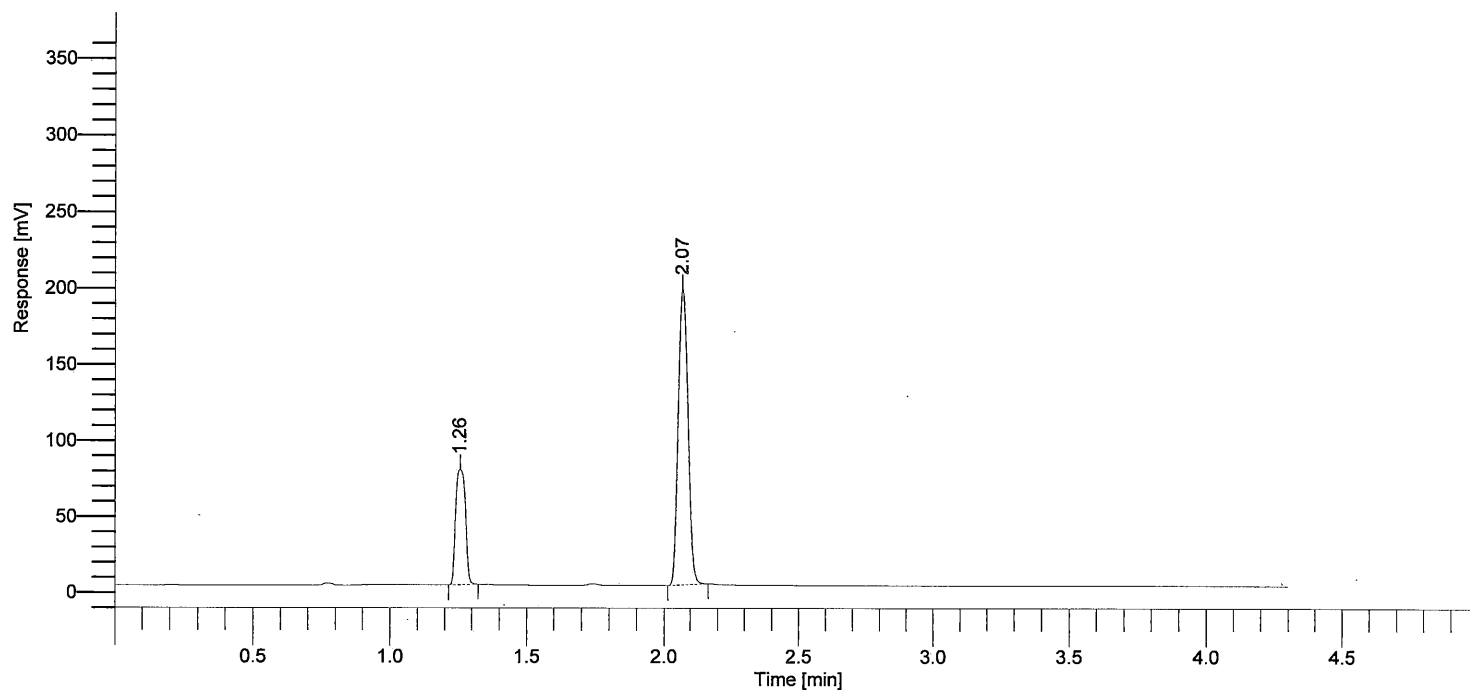

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.1204	1.26	188332.5
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	518687.3

34 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36865
Sample Name : GUTH 17390 #708
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 16

Date : 12/19/2017 10:25:39 AM
Data Acquisition Time : 12/19/2017 10:21:12 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-016.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

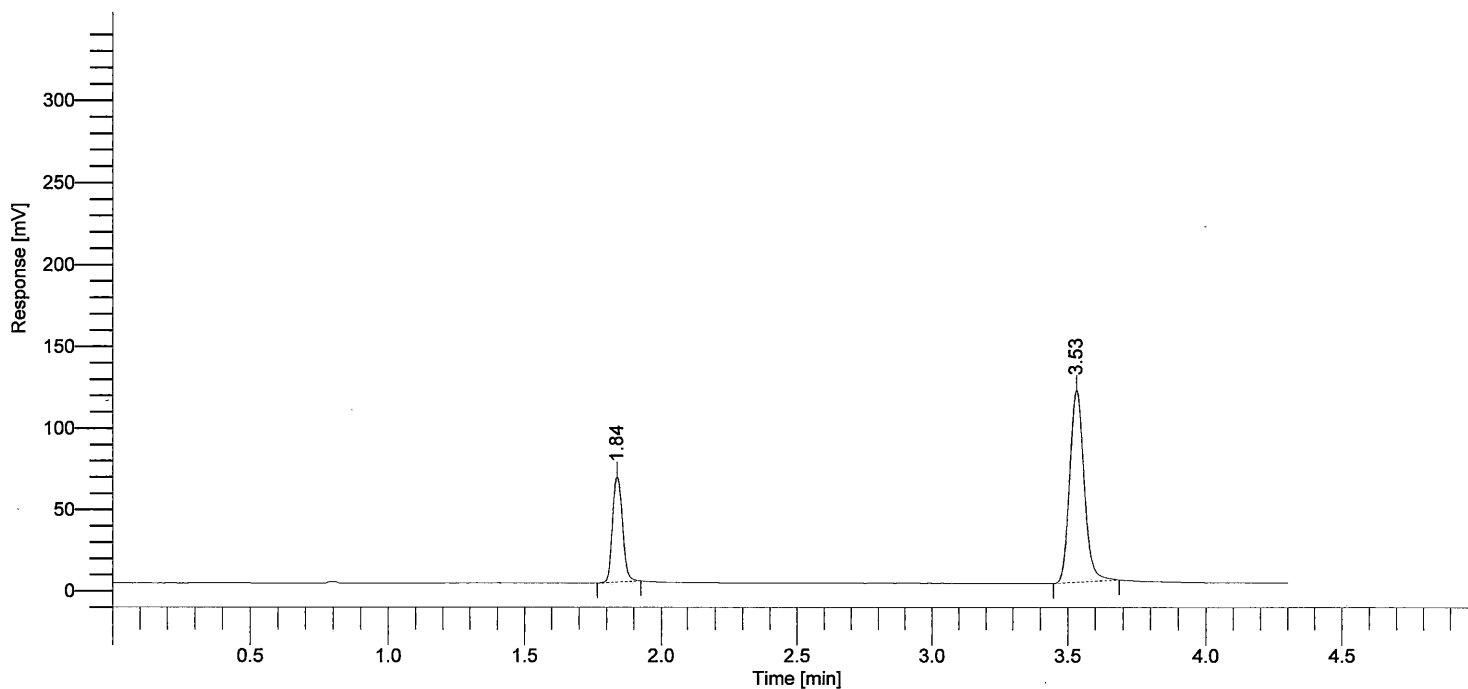

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

35 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36866
Sample Name : GUTH 17390 #708
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 17

Date : 12/19/2017 10:30:38 AM
Data Acquisition Time : 12/19/2017 10:26:12 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-017.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

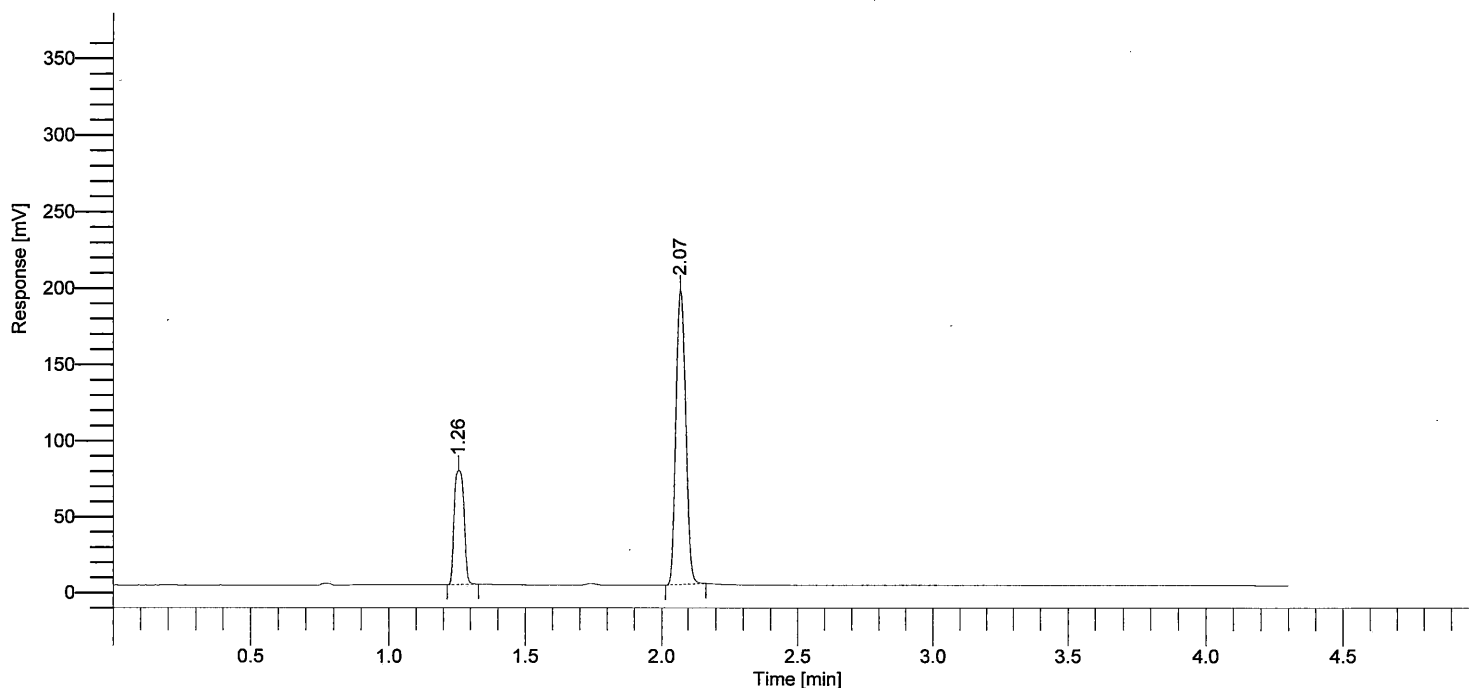

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [μ V·s]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.1207	1.26	187269.7
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	514675.8

36 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36867
Sample Name : GUTH 17390 #708
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 17

Date : 12/19/2017 10:30:40 AM
Data Acquisition Time : 12/19/2017 10:26:12 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-017.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

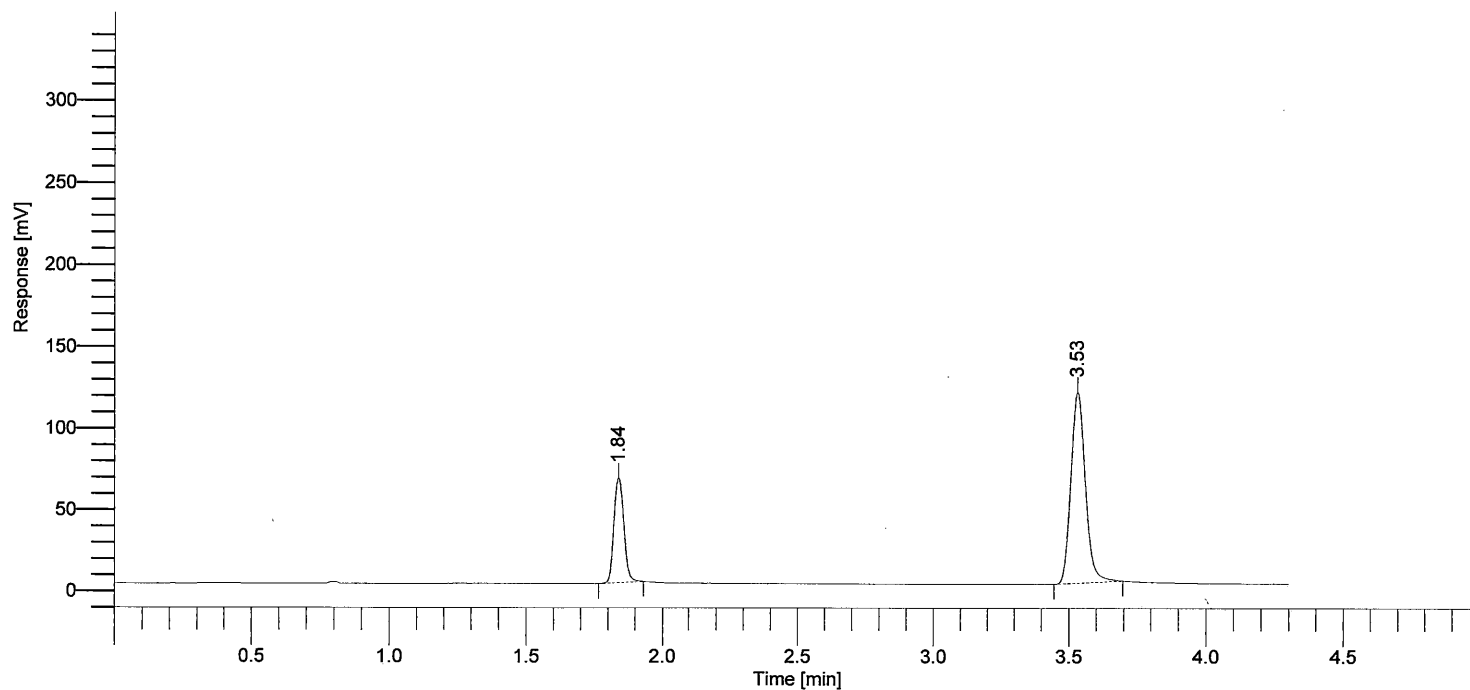

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

37 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36868
Sample Name : GUTH 17390 #708
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 18

Date : 12/19/2017 10:35:38 AM
Data Acquisition Time : 12/19/2017 10:31:12 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-018.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

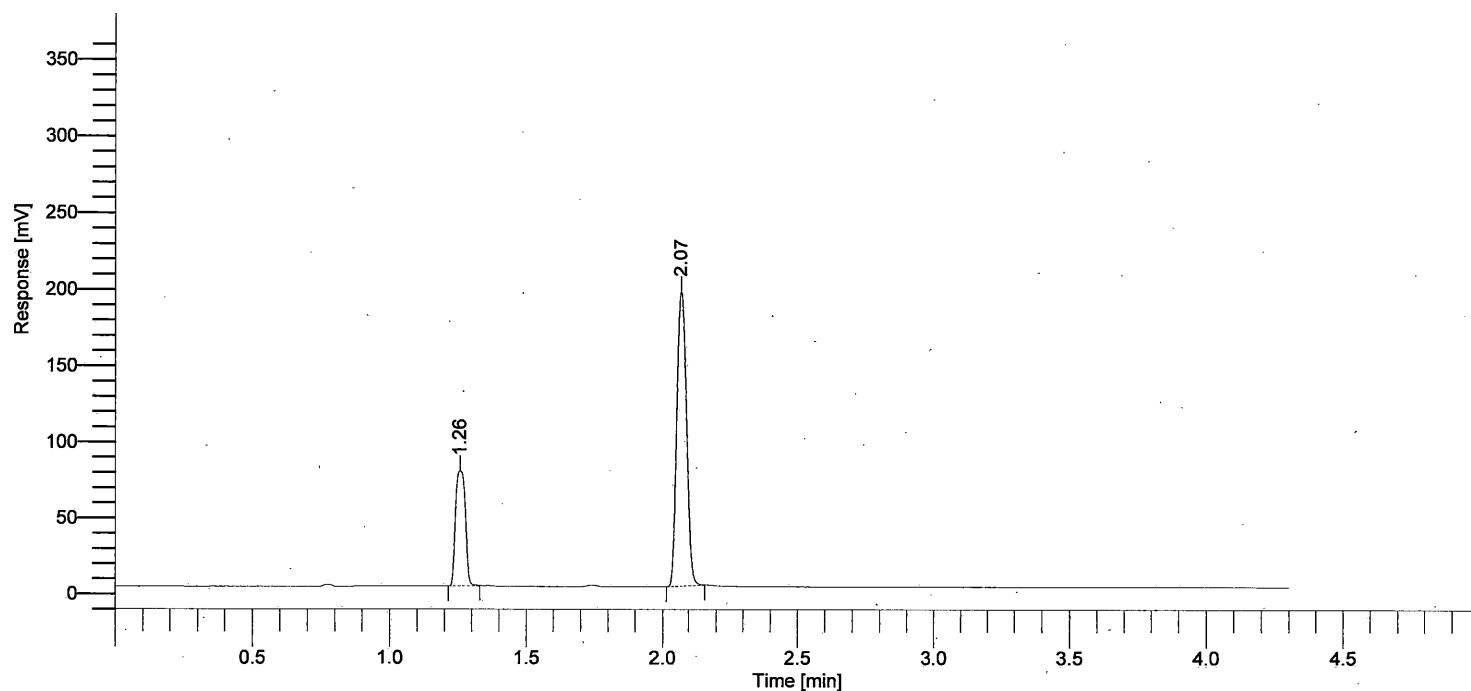

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.1206	1.26	188851.8
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	519234.0

38 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36869
Sample Name : GUTH 17390 #708
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 18

Date : 12/19/2017 10:35:39 AM
Data Acquisition Time : 12/19/2017 10:31:12 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-018.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

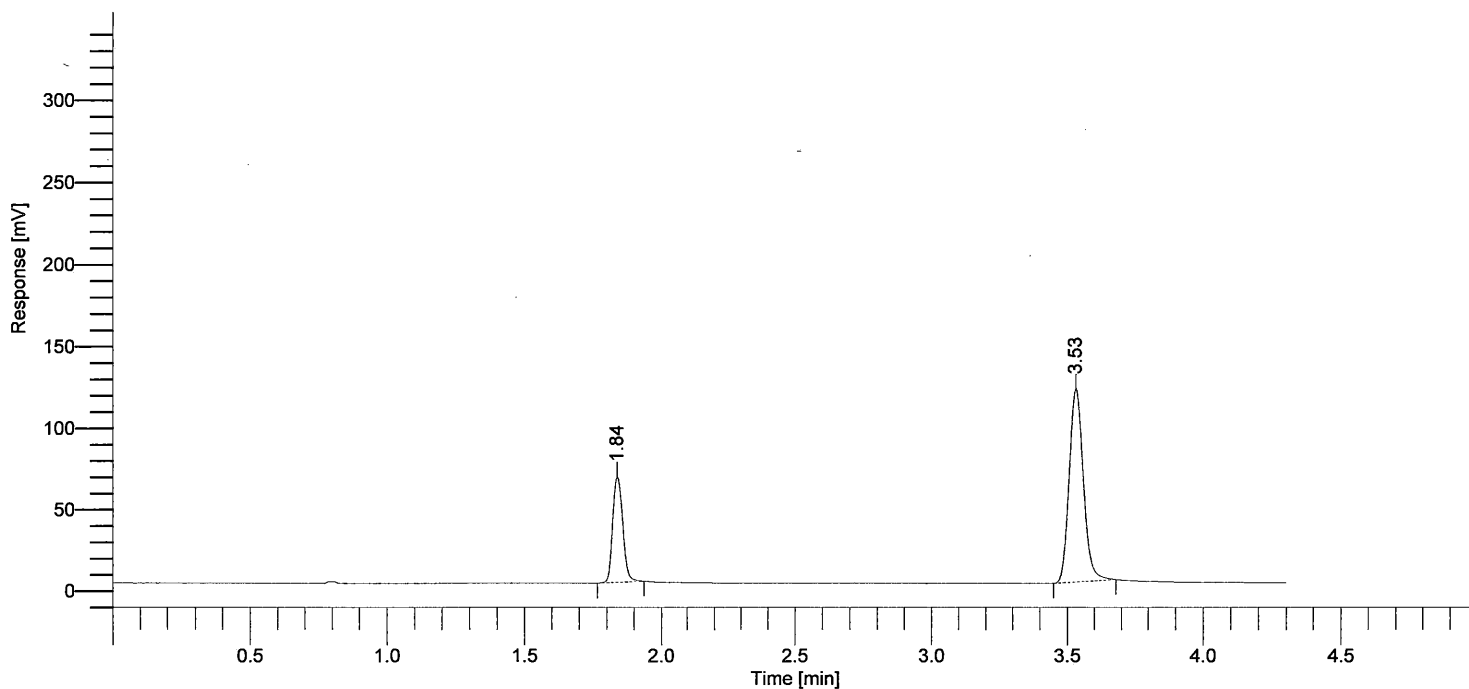

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

39 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36870
Sample Name : GUTH 17390 #1392
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 19

Date : 12/19/2017 10:40:38 AM
Data Acquisition Time : 12/19/2017 10:36:12 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-019.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

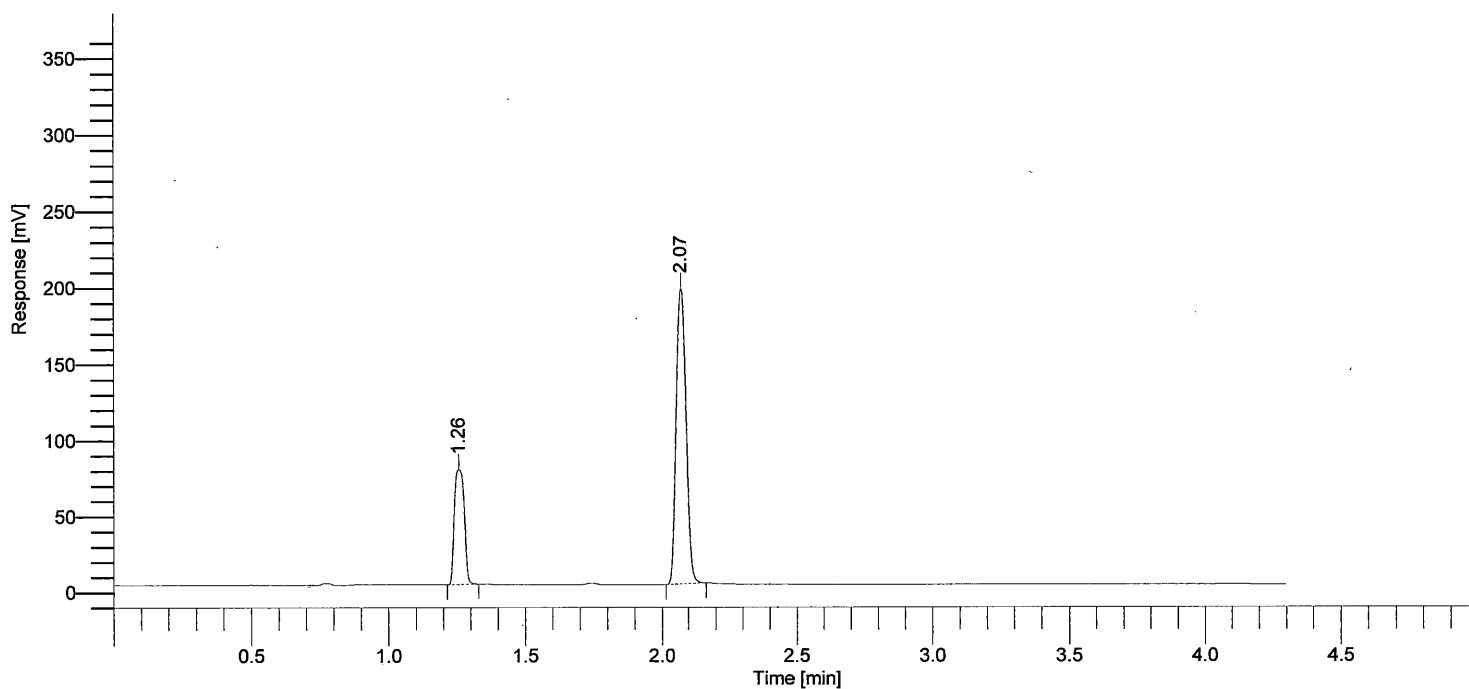

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.1205	1.26	189048.9
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	520472.3

40 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36871
Sample Name : GUTH 17390 #1392
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 19

Date : 12/19/2017 10:40:39 AM
Data Acquisition Time : 12/19/2017 10:36:12 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-019.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

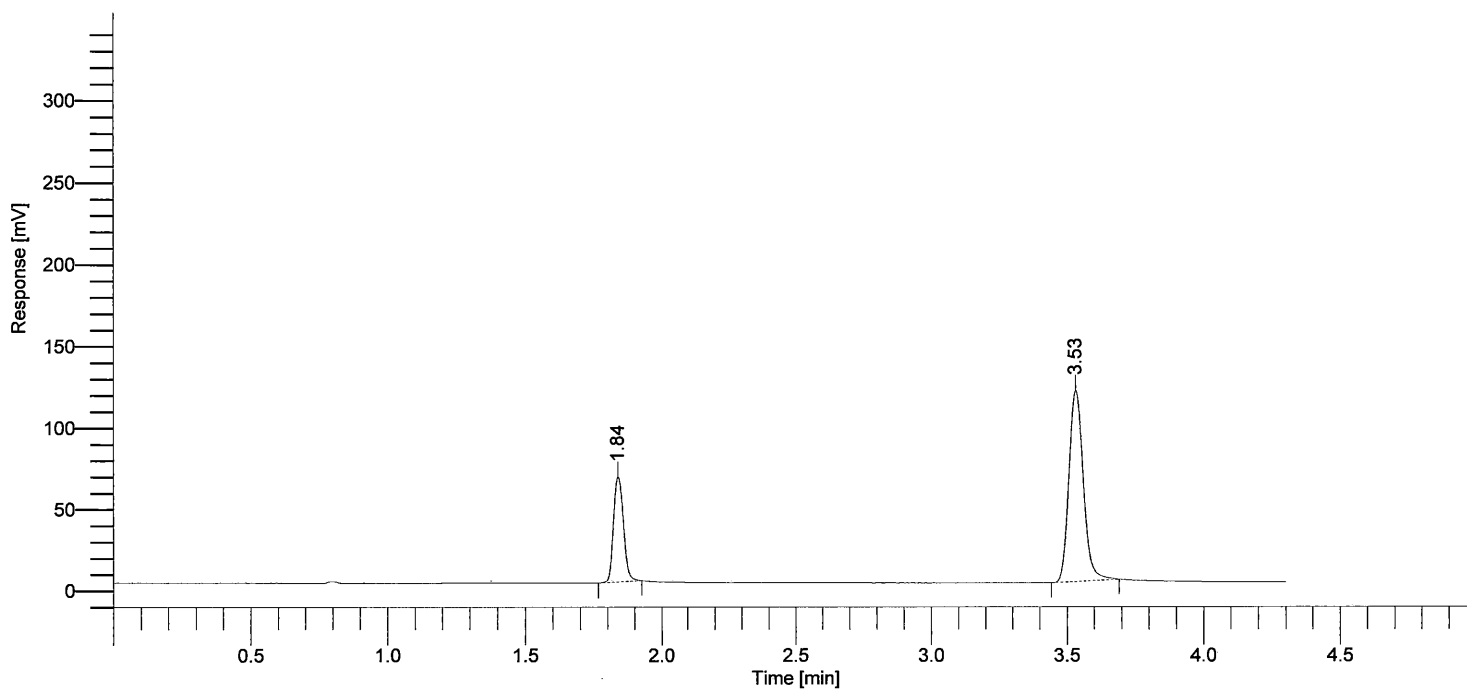

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

41 cm
~~41 cm~~ cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36872
Sample Name : GUTH 17390 #1392
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 20

Date : 12/19/2017 10:45:38 AM
Data Acquisition Time : 12/19/2017 10:41:12 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-020.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

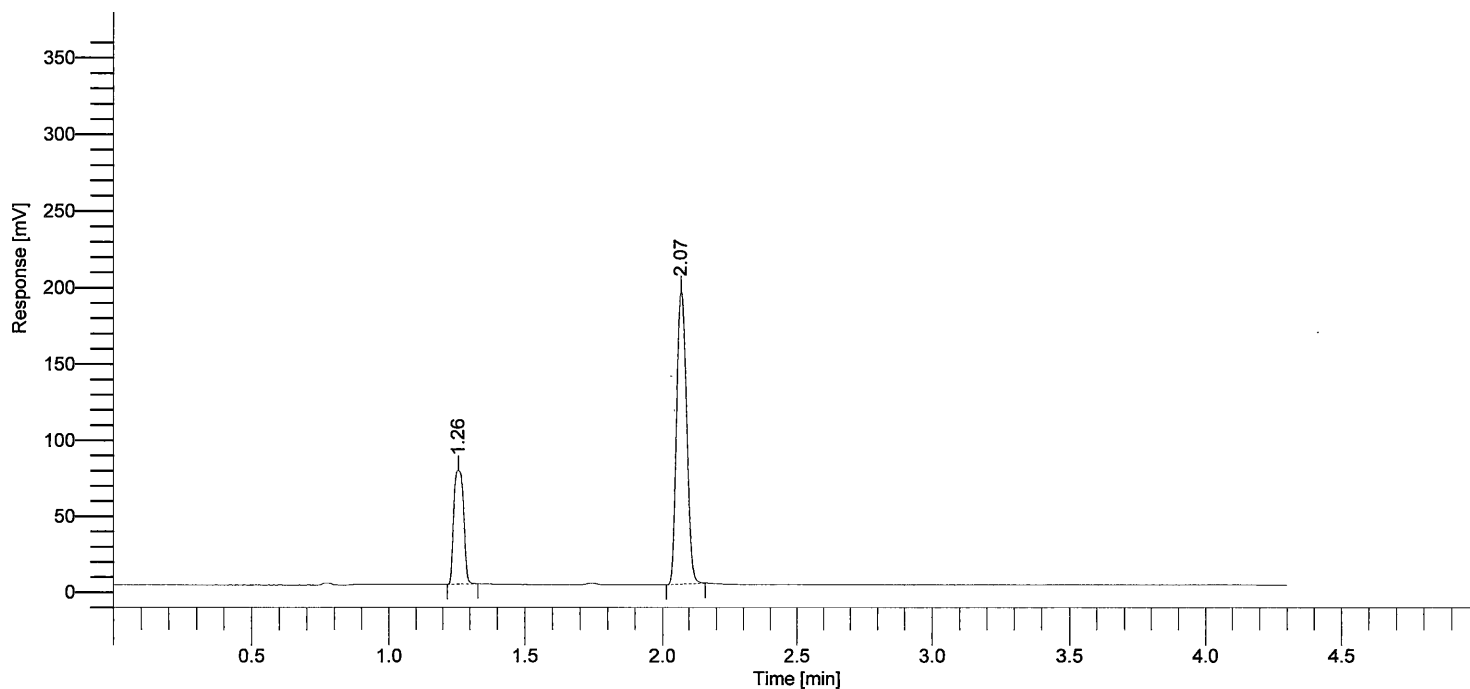

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [μ V·s]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.1208	1.26	186635.0
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	512514.6

42 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36873
Sample Name : GUTH 17390 #1392
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 20

Date : 12/19/2017 10:45:39 AM
Data Acquisition Time : 12/19/2017 10:41:12 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-020.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

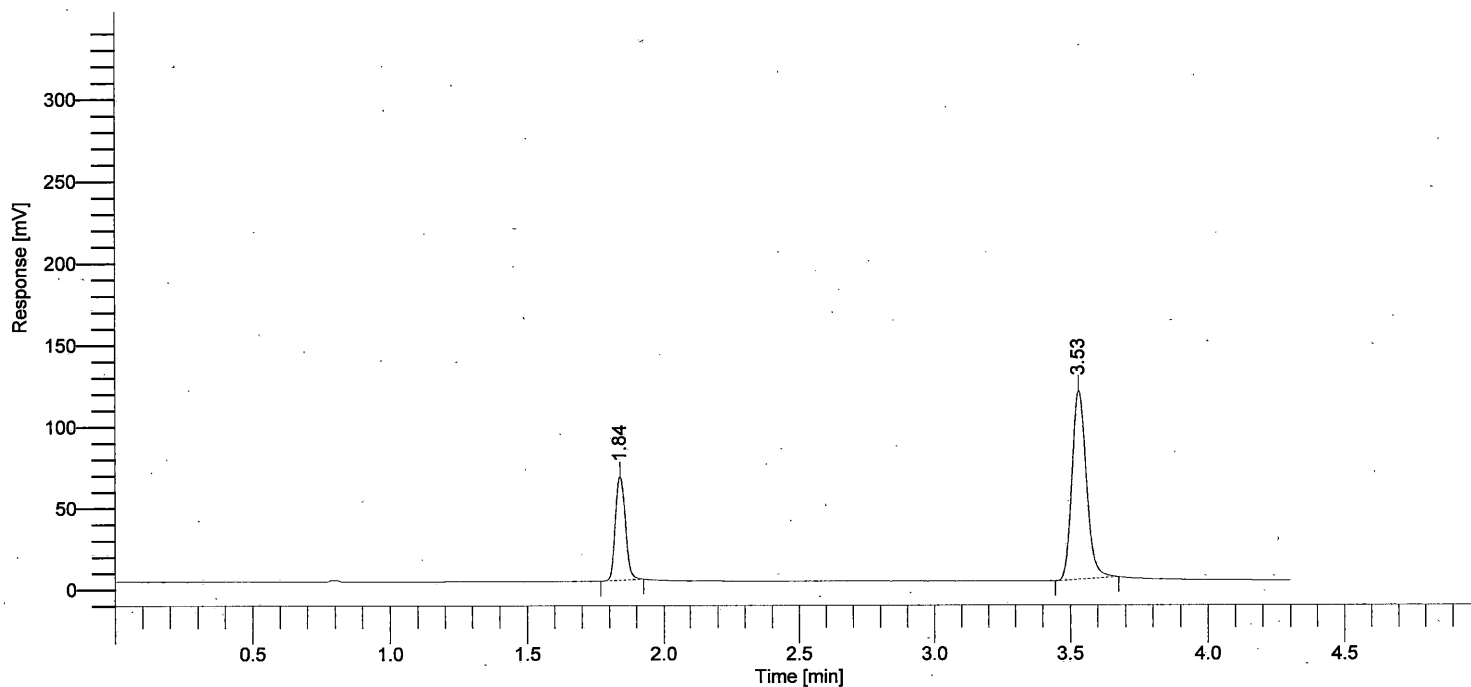

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

43 *cm*

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36874
Sample Name : GUTH 17390 #1392
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 21

Date : 12/19/2017 10:50:38 AM
Data Acquisition Time : 12/19/2017 10:46:12 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-021.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

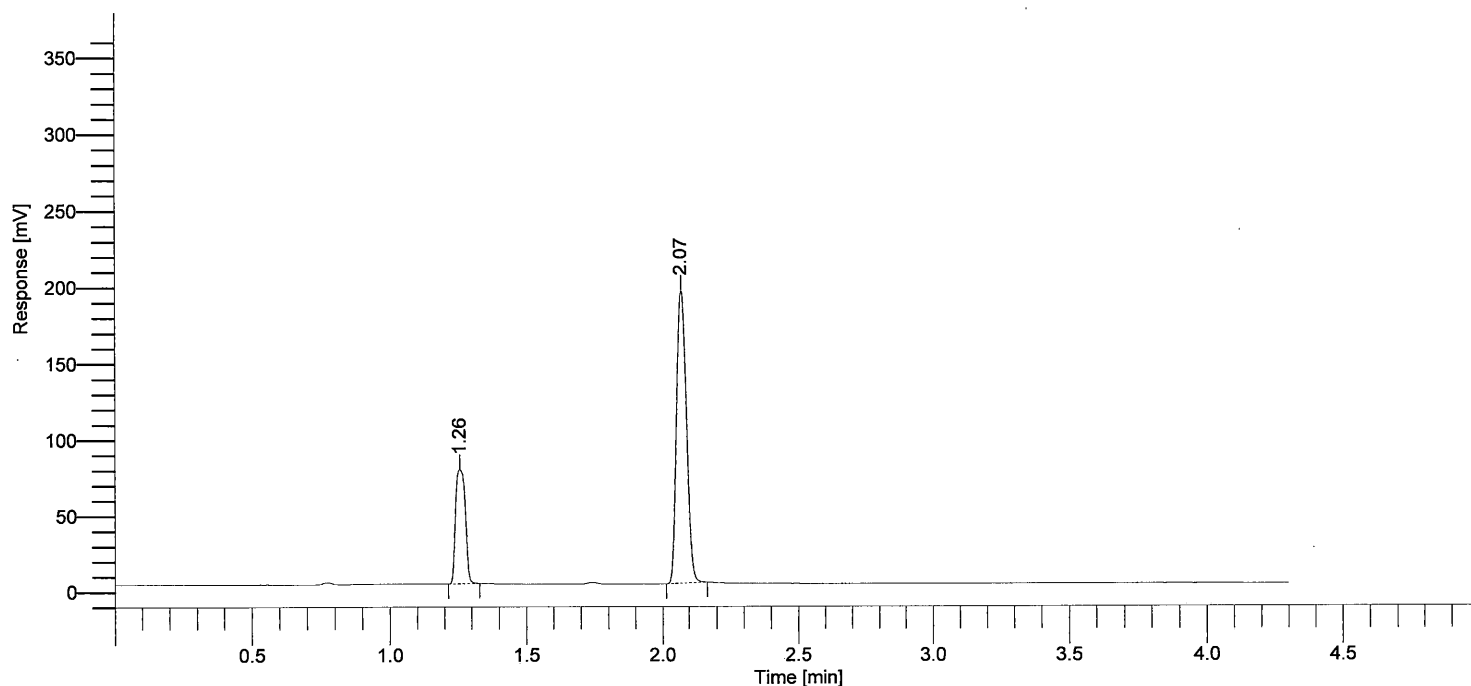

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.1209	1.26	186776.2
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	512300.3

44 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36875
Sample Name : GUTH 17390 #1392
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 21

Date : 12/19/2017 10:50:39 AM
Data Acquisition Time : 12/19/2017 10:46:12 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-021.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

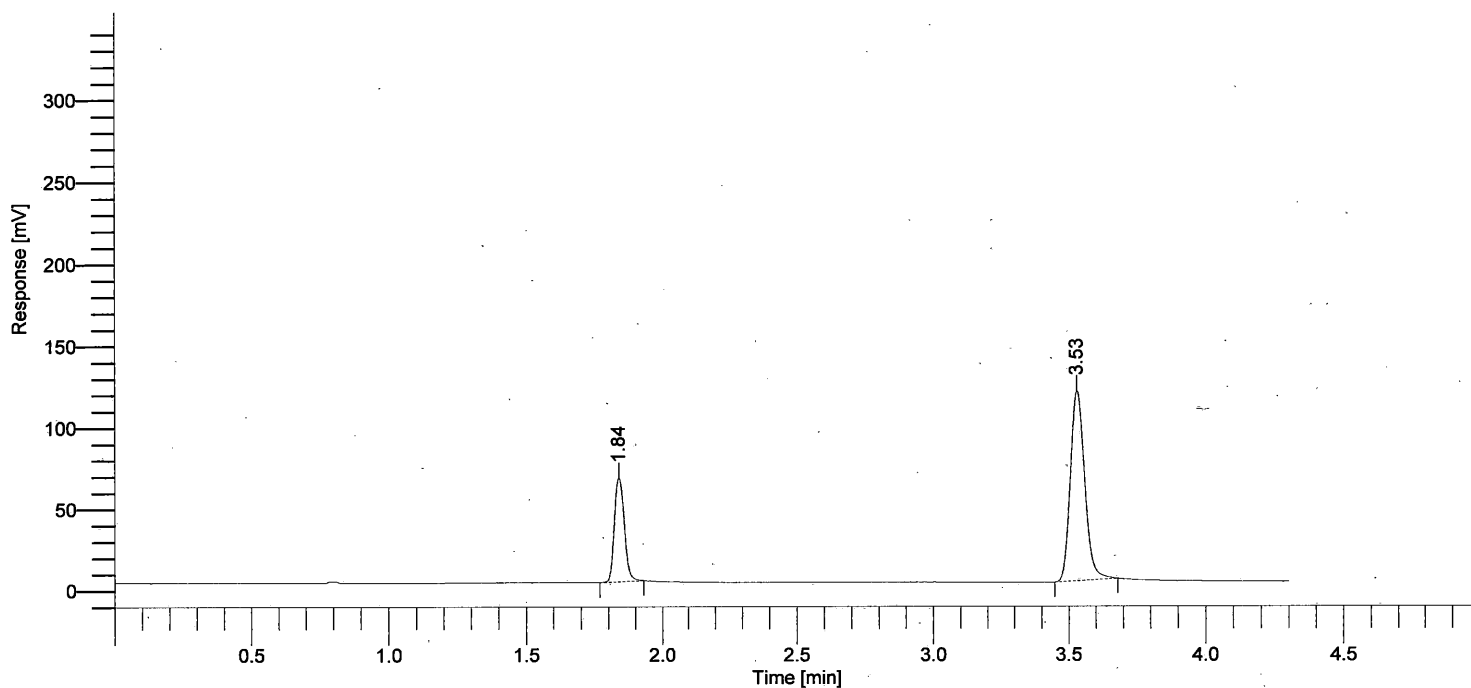

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

45 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36876
Sample Name : GUTH 17390 #1393
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 22

Date : 12/19/2017 10:55:35 AM
Data Acquisition Time : 12/19/2017 10:51:10 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-022.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

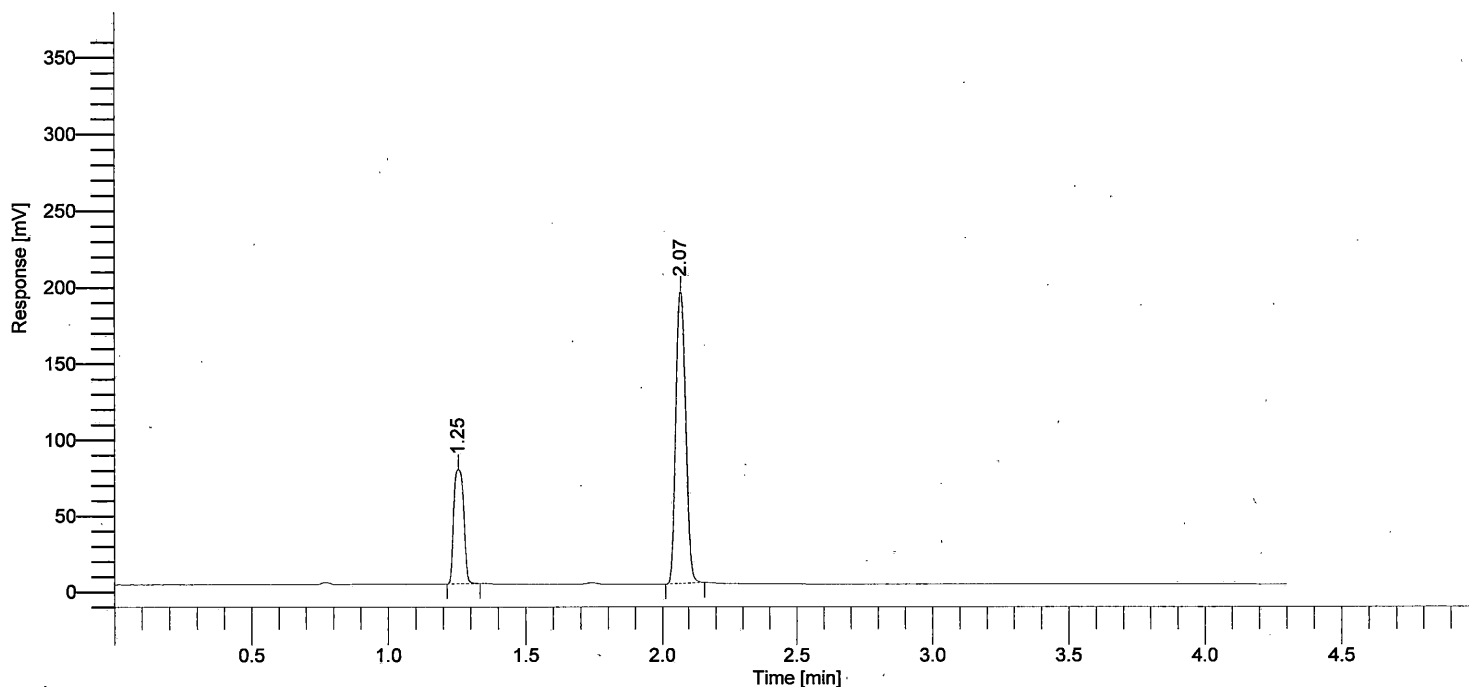

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [μ V·s]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.1212	1.25	188571.0
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	516055.2

46 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36877
Sample Name : GUTH 17390 #1393
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 22

Date : 12/19/2017 10:55:36 AM
Data Acquisition Time : 12/19/2017 10:51:10 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-022.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

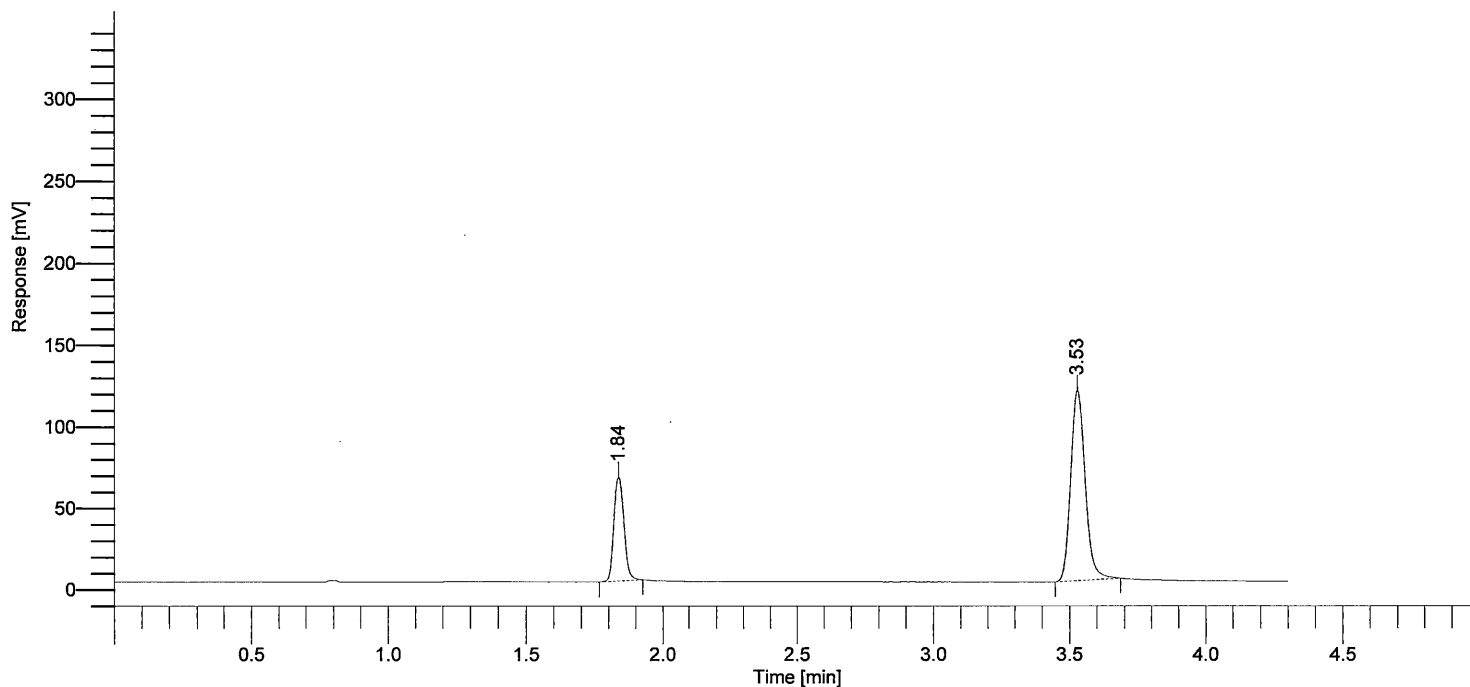

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

47 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36878
Sample Name : GUTH 17390 #1393
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 23

Date : 12/19/2017 11:00:35 AM
Data Acquisition Time : 12/19/2017 10:56:10 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-023.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

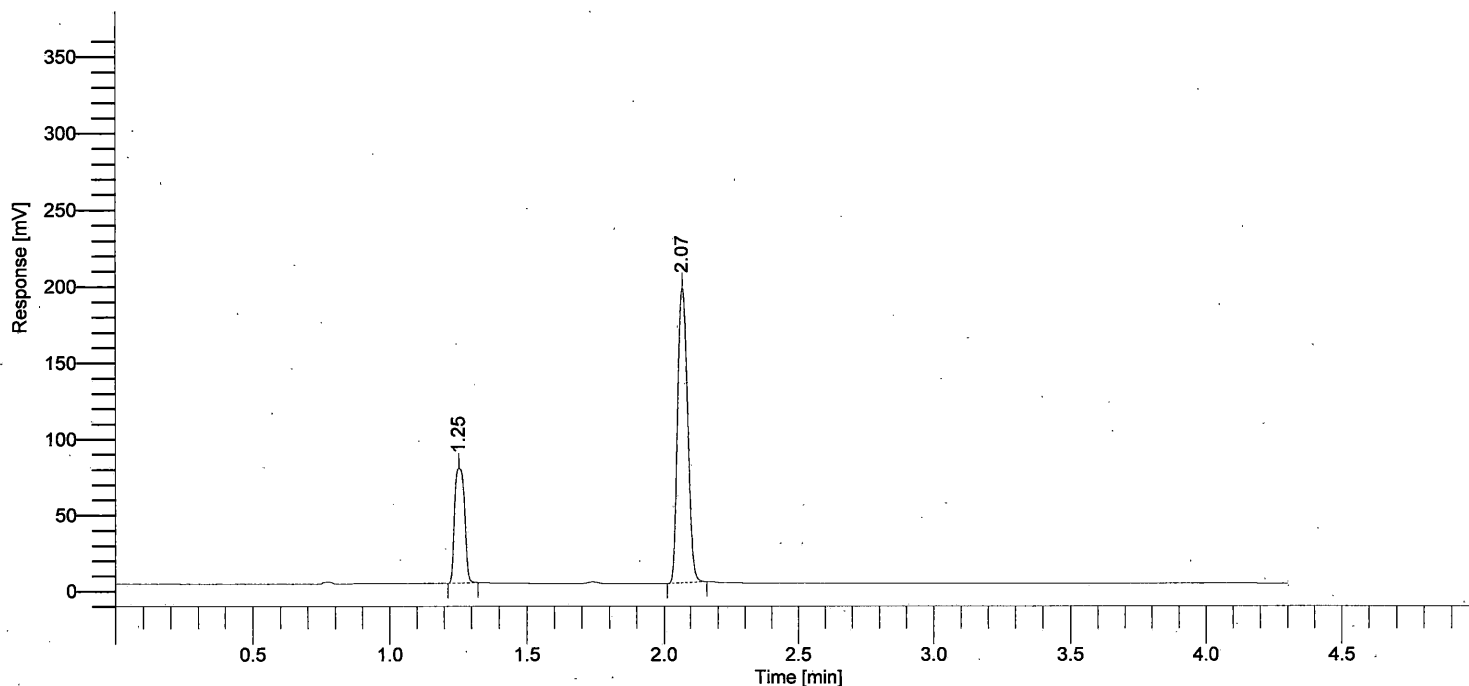

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [μ V·s]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.1207	1.25	189548.7
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	520929.5

48 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36879
Sample Name : GUTH 17390 #1393
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 23

Date : 12/19/2017 11:00:36 AM
Data Acquisition Time : 12/19/2017 10:56:10 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-023.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

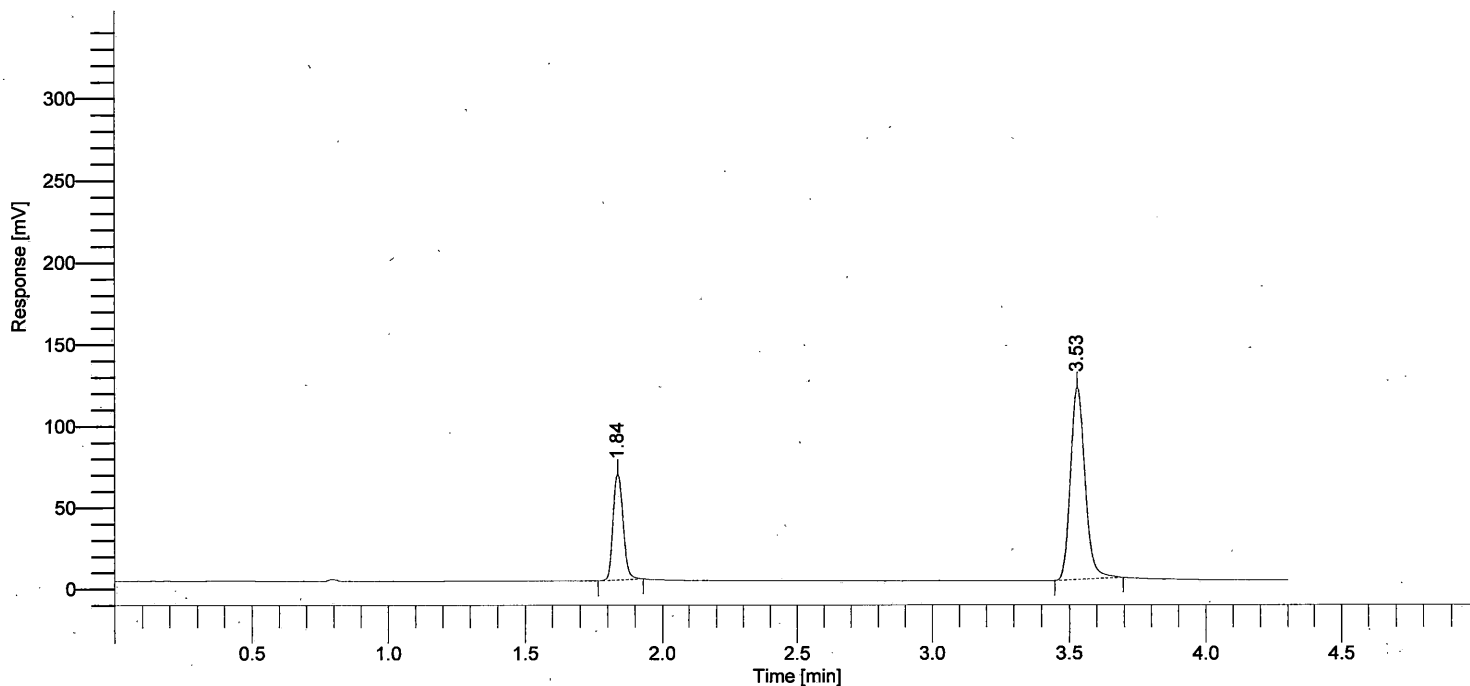

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

49 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36880
Sample Name : GUTH 17390 #1393
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 24

Date : 12/19/2017 11:05:35 AM
Data Acquisition Time : 12/19/2017 11:01:10 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-024.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

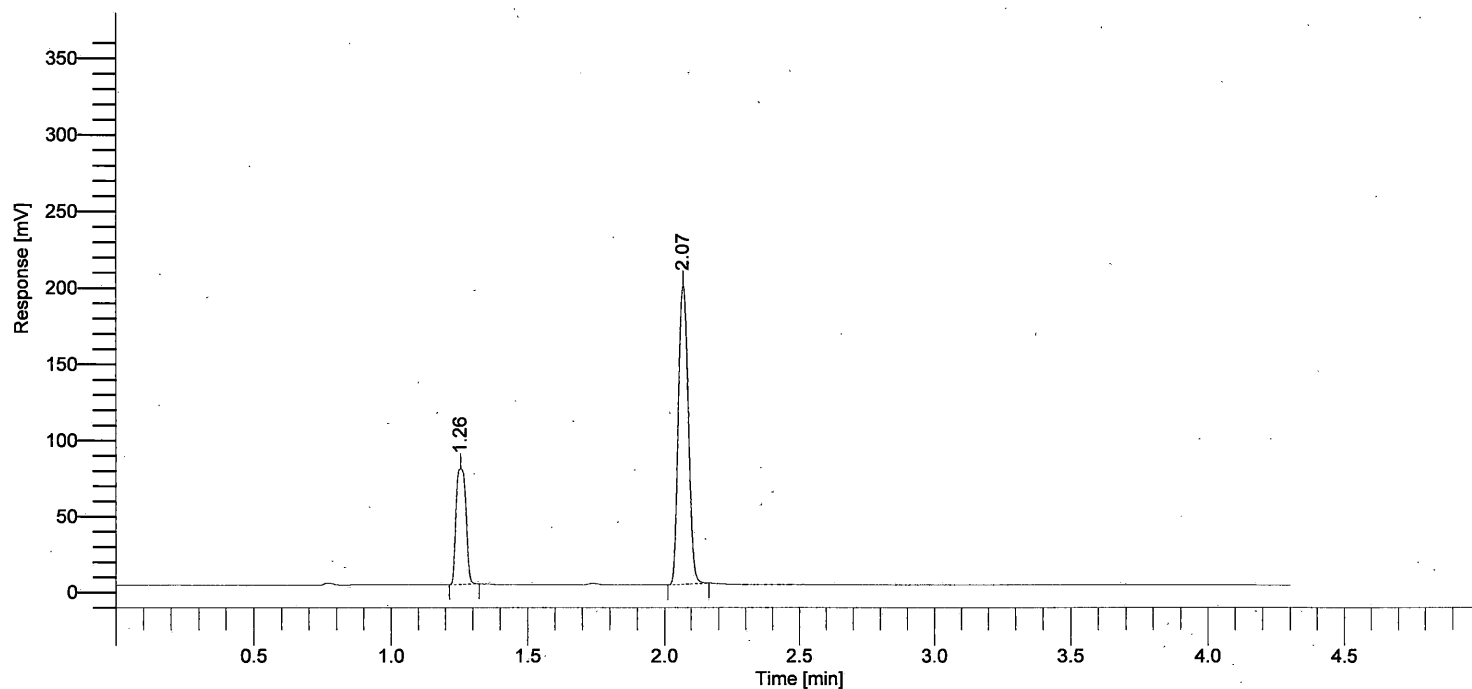

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.1202	1.26	191653.9
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	528588.3

50 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36881
Sample Name : GUTH 17390 #1393
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 24

Date : 12/19/2017 11:05:37 AM
Data Acquisition Time : 12/19/2017 11:01:10 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-024.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

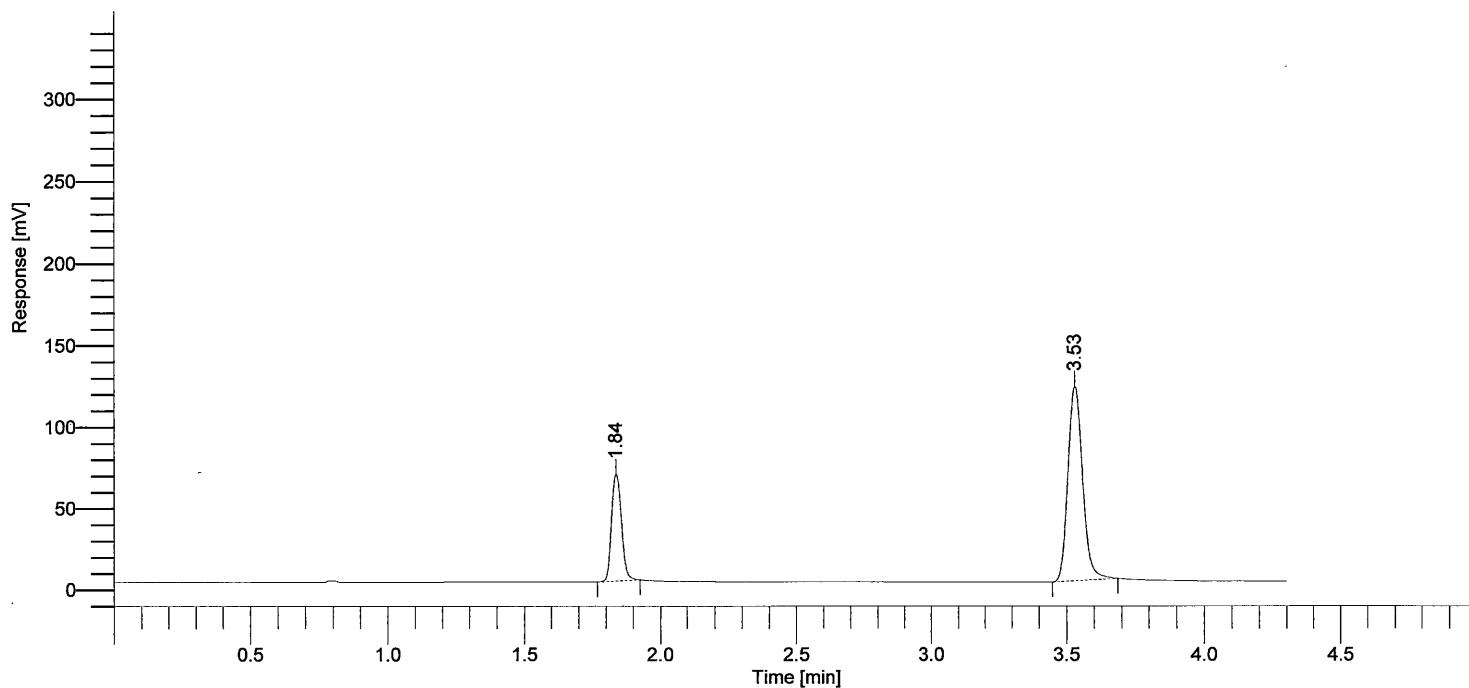

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

51 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36882
Sample Name : 0.10% CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 25

Date : 12/19/2017 11:10:35 AM
Data Acquisition Time : 12/19/2017 11:06:10 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-025.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

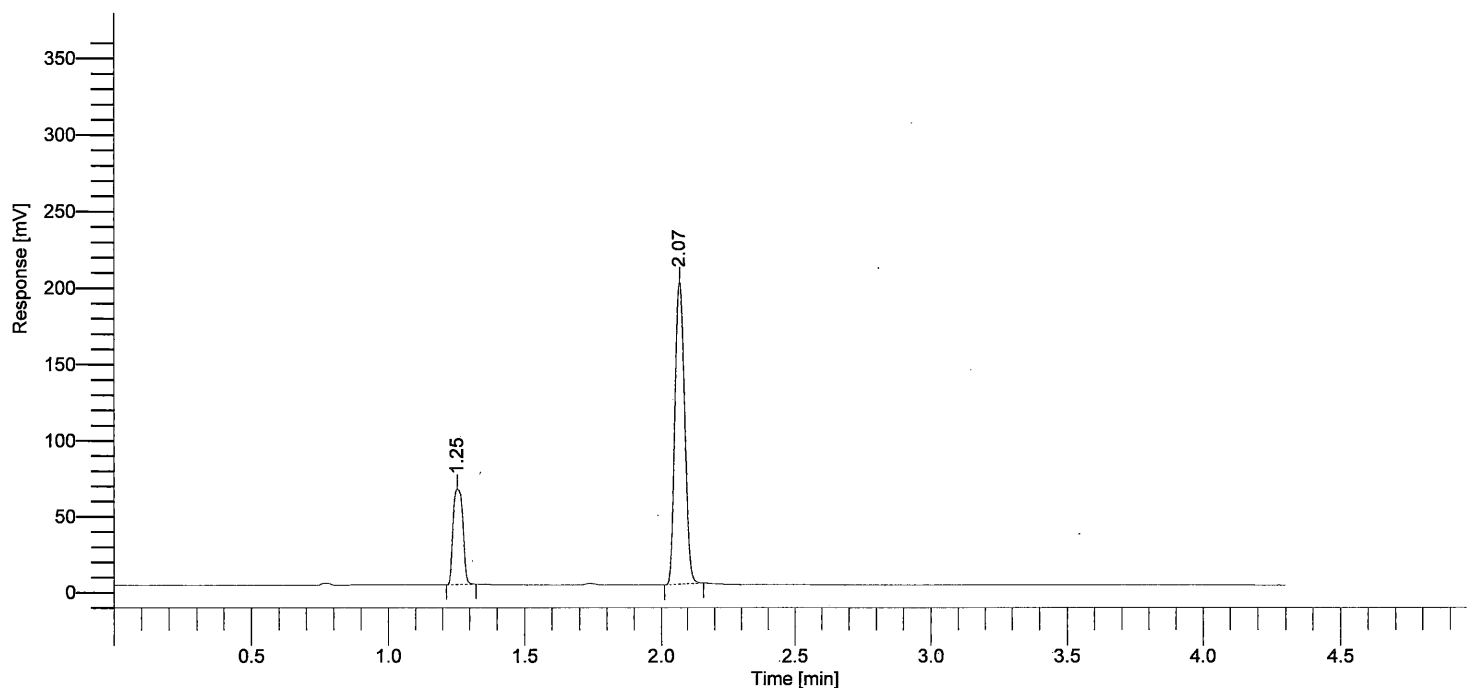

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.0986	1.25	157001.8
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	529843.2

S2 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36883
Sample Name : 0.10% CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 25

Date : 12/19/2017 11:10:36 AM
Data Acquisition Time : 12/19/2017 11:06:10 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-025.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

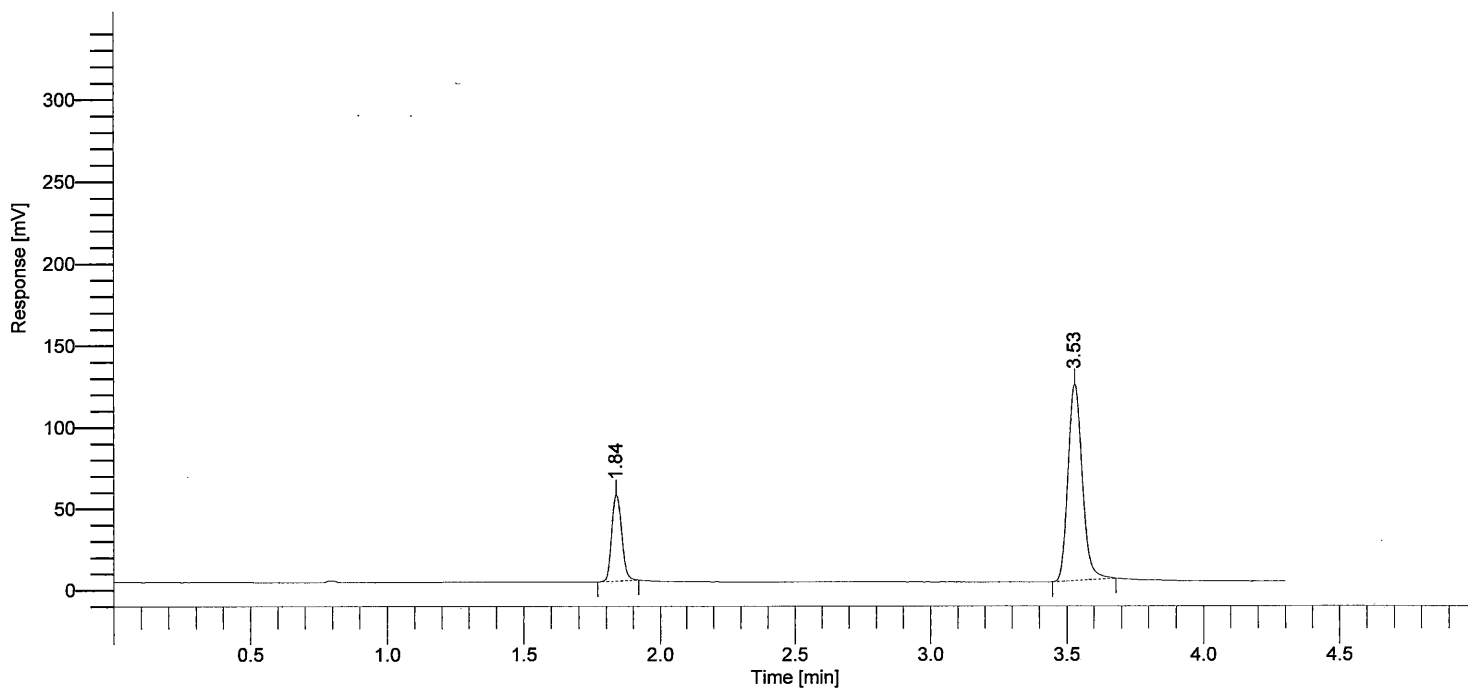

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

S3 *[signature]*

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36884
Sample Name : 0.20% CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 26

Date : 12/19/2017 11:15:35 AM
Data Acquisition Time : 12/19/2017 11:11:10 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-026.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

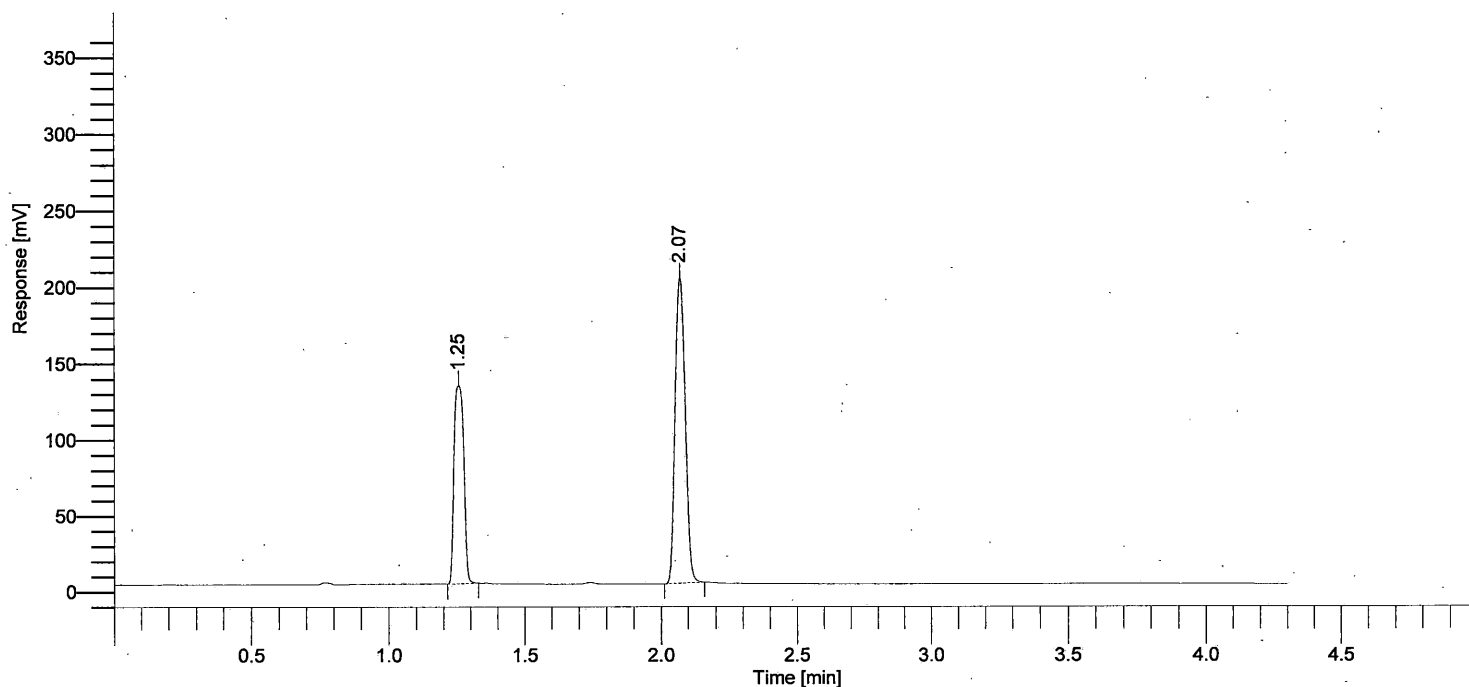

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.1992	1.25	325250.5
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	538465.2

54 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36885
Sample Name : 0.20% CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 26

Date : 12/19/2017 11:15:37 AM
Data Acquisition Time : 12/19/2017 11:11:10 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-026.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

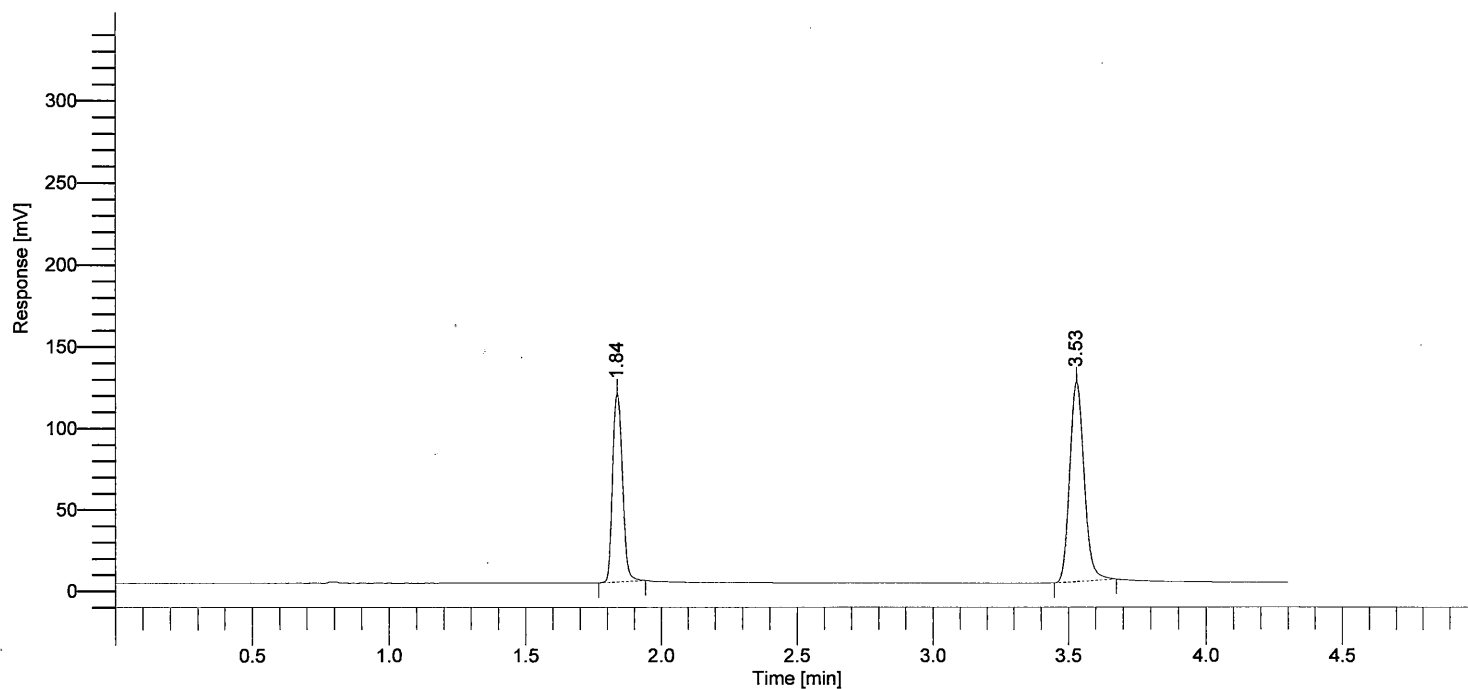

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.84
N-PROPANOL	3.53

SS cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36886
Sample Name : NEG CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 27

Date : 12/19/2017 11:20:35 AM
Data Acquisition Time : 12/19/2017 11:16:10 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20171219-027.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

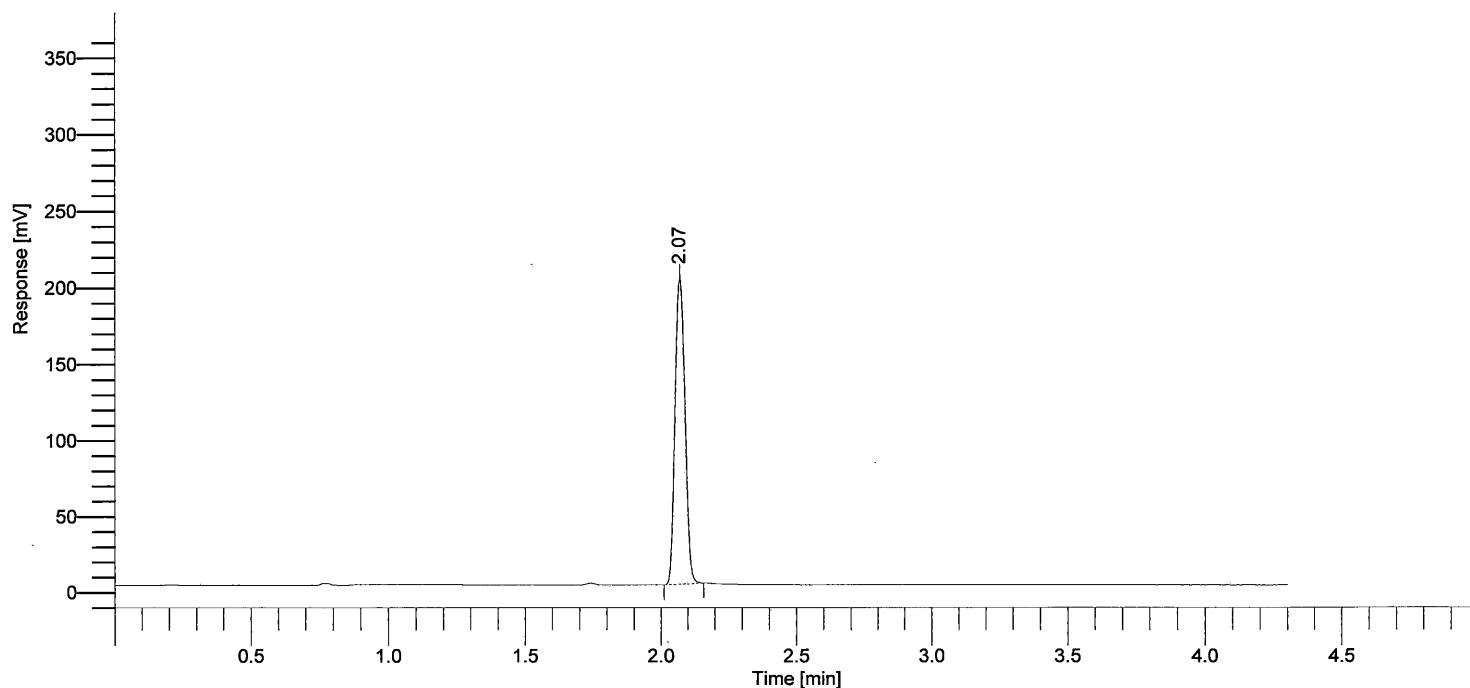

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.00	0.0
ETHANOL	0.0000	1.26	0.0
ISOPROPANOL	0.0000	1.54	0.0
ACETONE	0.0000	1.90	0.0
N-PROPANOL	-----	2.07	536638.6

56 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 36887
Sample Name : NEG CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 27

Date : 12/19/2017 11:20:36 AM
Data Acquisition Time : 12/19/2017 11:16:10 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20171219-027.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

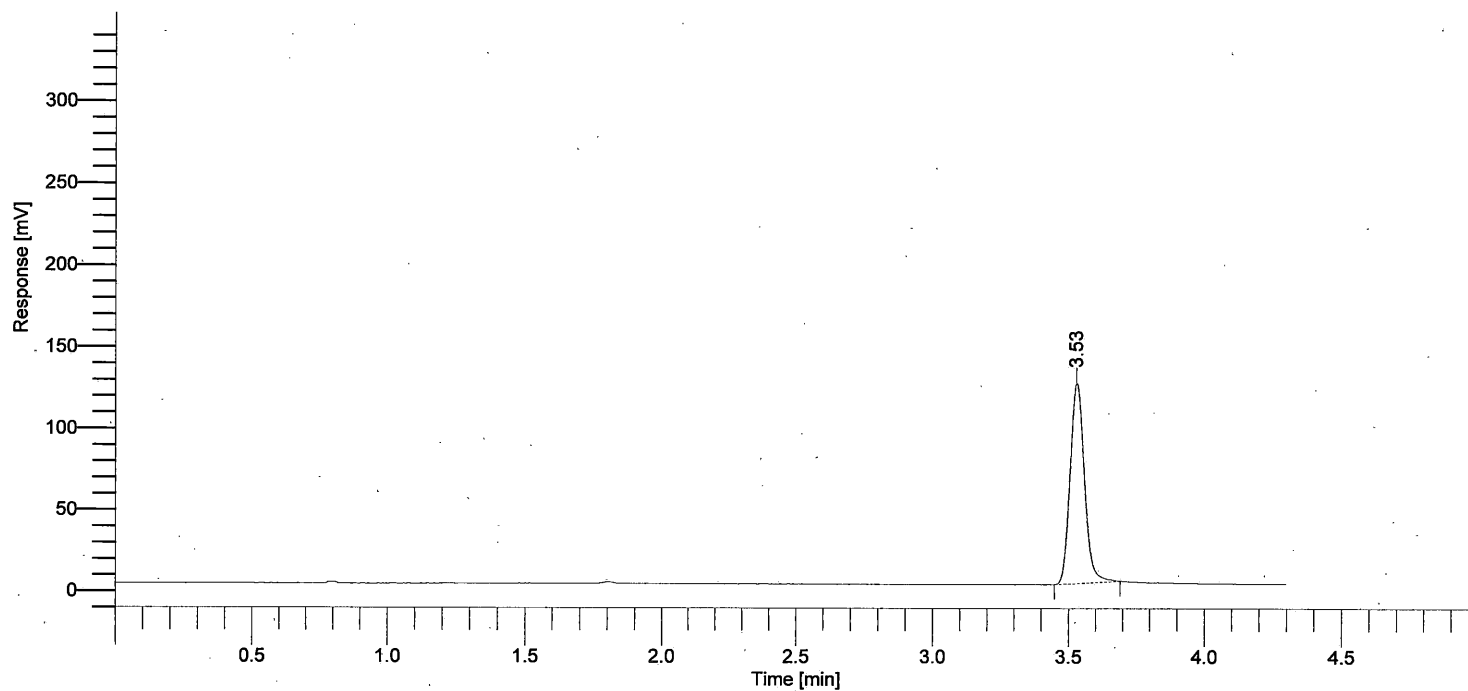

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"

Component Name	Time [min]
N-PROPANOL	3.53

57 cm