

New York State Police Crime Laboratory System
BREATH TESTING

Technical & Administrative Review Checklist - Simulator Solution

Class: Form
ID: Breath Form 4b (Version 6)

Effective Date: December 11, 2018
Page: 1 of 1

Solution Lot Number: 19130

Review Start Date: 6/17/19

Reviewer (initials): OA

Documentation:

- ☒ Handwritten initials on all pages
- ☒ Page number on all pages, total pages noted
- ☒ Solution lot number on all solution pages; bottle number on all analytical pages
- ☒ Proper sample loading documented
- ☒ All pages of the technical record were reviewed for corrections; if applicable, corrections were documented appropriately
- ☒ Dates of analyses documented
- ☒ If abbreviations/symbols specific to the laboratory are used, they have been defined in section procedures
- NA Any deviations from acceptability criteria have documented approval

Quality Control Data:

- ☒ Correct version of the test method is indicated on the QC Worksheet
- ☒ Required control samples analyzed, expiration dates not exceeded
- ☒ Acceptance criteria met
- ☒ QC results are accurately entered in Tox Form 11 QC Spreadsheet

Technical Data:

- ☒ The technical records demonstrate compliance with test methods
- ☒ Data transfers are accurate
- ☒ Retention times are recorded and acceptable
- ☒ Results meet acceptability criteria

Simulator Solution Record (electronic):

- ☒ Solution specific information is accurate (e.g. lot number, expiration date, etc)
- ☒ Results are accurately reported
- ☒ Electronic signature applied
- ☒ File name accurate

Review Completed:

- ☒ Upon review of the technical records available, I independently reached the same conclusion(s) reported.

Reviewer (initial/date): OA 6/17/19

Page 1 of 1

**New York State Police Crime Laboratory System
BREATH TESTING**

Simulator Solution Verification Results

Class: Form
ID: Breath Form 2 (Version 3)

Effective Date: June 1, 2015
Page: 1 of 1

Simulator Solution Level: 0.10 %

Target Concentration: 0.121 %
Acceptable Range: 0.117-0.125 %

Manufacturer: Guth Laboratories, Inc.
Lot Number: 19130

Analyst: Carol S Miller
Analysis Date: 6/13/2019

Bottle Number	% by wt	AVG
8	0.1195 0.1192 0.1190	0.1192
9	0.1191 0.1189 0.1183	0.1188
732	0.1189 0.1195 0.1189	0.1191
733	0.1193 0.1194 0.1194	0.1194
1445	0.1193 0.1197 0.1191	0.1194
1446	0.1189 0.1218 0.1194	0.1200
Grand Average		0.1193

pg 1 of 57

New York State Police Crime Laboratory System
BREATH TESTING

Simulator Solution Verification QC Worksheet

Class: Form
ID: Breath Form 8 (Version 2)

Effective Date: January 10, 2017
Page: 1 of 1

Analysis Date: 06-13-19
Analyst Initials: Cam

Breath Instr 2 Version 6

Simulator Solution Lot# 19130

Expiration Date 11-28-19
Received Date 06-10-19
Level 0.10%
Bottle Number(s) 8, 9, 732, 733, ~~1443, 1444~~ 1445, 1446

<u>Internal Standard</u>	<u>Lot #</u>	<u>Expiration Date</u>
n-propanol	<u>SWL060619</u>	<u>09-06-19</u>

<u>Controls</u>	<u>Lot #</u>	<u>Expiration Date</u>
0.08 % by wt	<u>FN04171701</u>	<u>05/2022</u>
0.10 % by wt	<u>FN02271802</u>	<u>04/2023</u>
0.20 % by wt	<u>FN06231704</u>	<u>08/2022</u>
0.30 % by wt	<u>NA</u>	<u>NA</u>
0.40 % by wt	<u>NA</u>	<u>NA</u>
0.50 % by wt	<u>NA</u>	<u>NA</u>
Composite	<u>SWL013019</u>	<u>01-30-20</u>

<u>Instrumentation</u>	<u>Instrument ID/Serial #</u>	<u>Calibration Exp Date</u>
Headspace GC	<u>H-TX-H52</u>	<u>09-06-19</u>
Dilutor	<u>MD965E622</u>	<u>09-30-19</u>

Test Method Analyst Review

Batch Accepted ☒ Batch Rejected ☐

Rejection reason/course of action: _____

Deviations/departures: _____

Comments: _____

Initial/Date: Cam 06-14-19 2 Cam

Approved By: Top Management

Print Date: 6/13/2019

TotalChrom Sequence File C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

Printed by : manager on: 6/13/2019 8:33:20 AM
Created by : toxicology on: 8/6/2009 1:12:05 PM
Edited by : manager on: 6/13/2019 8:33:18 AM
Number of Times Edited : 66

Description:

Sequence File Header Information:

Number of Rows : 27
Instrument Type : PE AutoSystem GC
Injection Type : SINGLE
Raw tokens channel A :
Result tokens channel A :
Modified tokens channel A :
Raw tokens channel B :
Result tokens channel B :
Modified tokens channel B :

Sequence Sample Descriptions - Channel A

Row	Type	Name
✓ 1	Sample	COMPOSITE ✓
✓ 2	Sample	0.08% CONTROL ✓
✓ 3	Sample	0.10% CONTROL ✓
✓ 4	Sample	NEG CONTROL ✓
✓ 5	Sample	GUTH 19130 #8 ✓
✓ 6	Sample	GUTH 19130 #8 ✓
✓ 7	Sample	GUTH 19130 #8 ✓
✓ 8	Sample	GUTH 19130 #9 ✓
✓ 9	Sample	GUTH 19130 #9 ✓
✓ 10	Sample	GUTH 19130 #9 ✓
✓ 11	Sample	GUTH 19130 #732 ✓
✓ 12	Sample	GUTH 19130 #732 ✓
✓ 13	Sample	GUTH 19130 #732 ✓
✓ 14	Sample	0.10% CONTROL ✓
✓ 15	Sample	NEG CONTROL ✓
✓ 16	Sample	GUTH 19130 #733 ✓
✓ 17	Sample	GUTH 19130 #733 ✓
✓ 18	Sample	GUTH 19130 #733 ✓
✓ 19	Sample	GUTH 19130 #1445 ✓
✓ 20	Sample	GUTH 19130 #1445 ✓
✓ 21	Sample	GUTH 19130 #1445 ✓
✓ 22	Sample	GUTH 19130 #1446 ✓
✓ 23	Sample	GUTH 19130 #1446 ✓
✓ 24	Sample	GUTH 19130 #1446 ✓
✓ 25	Sample	0.10% CONTROL ✓
✓ 26	Sample	0.20% CONTROL ✓
✓ 27	Sample	NEG CONTROL ✓

CM
06-13-19


HTG
6/13/19

3CM

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53451
Sample Name : COMPOSITE
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 1

Date : 6/13/2019 9:20:35 AM
Data Acquisition Time : 6/13/2019 9:16:10 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-001.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

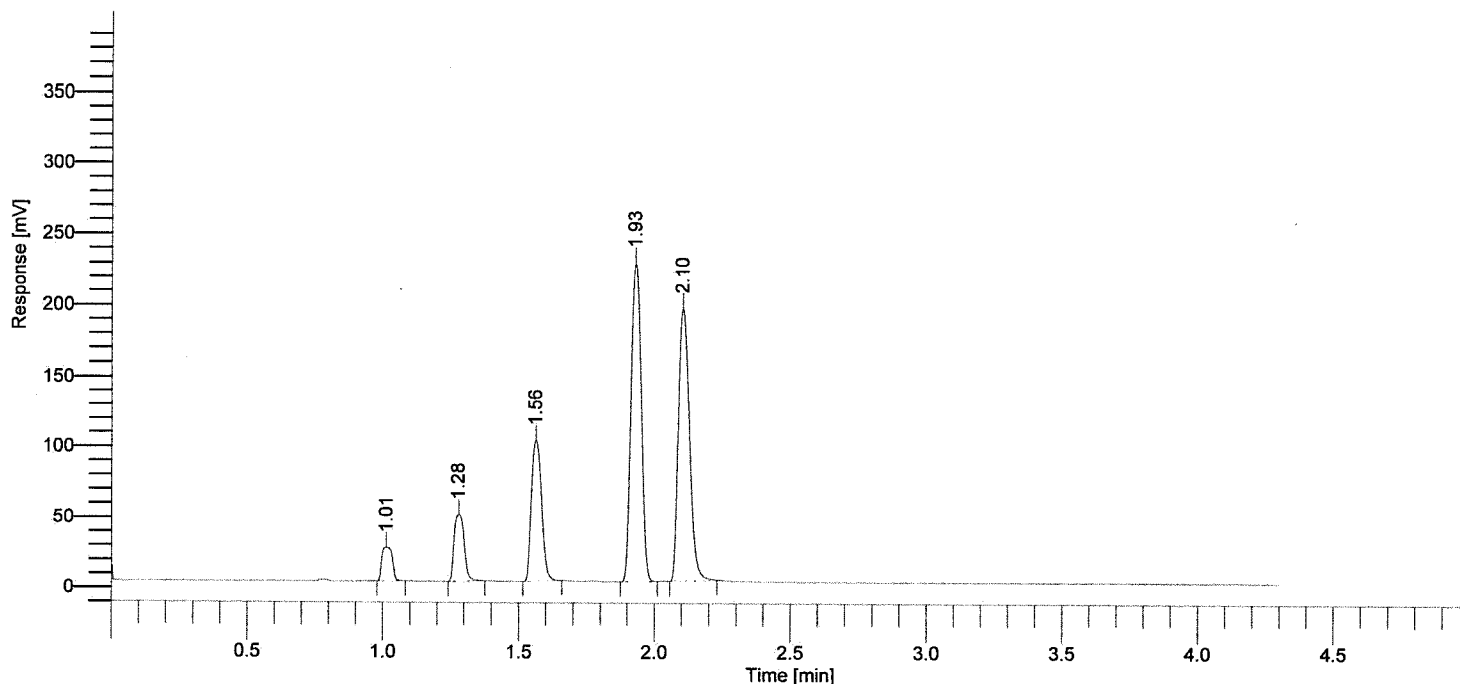

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0774	1.01	63853.1
ETHANOL	0.0783	1.28	125001.8
ISOPROPANOL	0.0800	1.56	261278.3
ACETONE	0.0781	1.93	587040.5
N-PROPANOL	-----	2.10	547496.7

4Cem

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53452
Sample Name : COMPOSITE
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 1

Date : 6/13/2019 9:20:37 AM
Data Acquisition Time : 6/13/2019 9:16:10 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-001.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

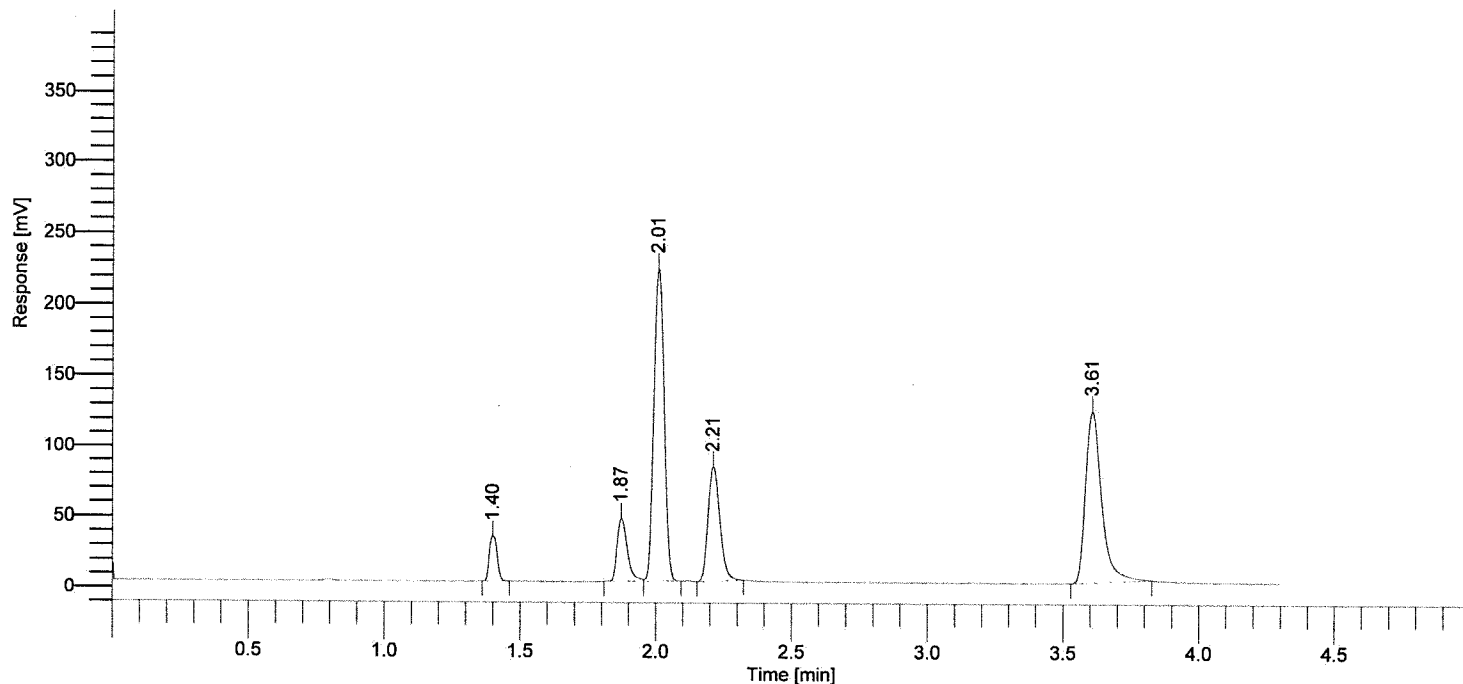

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
METHANOL	1.40
ETHANOL	1.87
ACETONE	2.01
ISOPROPANOL	2.21
N-PROPANOL	3.61

5 C

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53453
Sample Name : 0.08% CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 2

Date : 6/13/2019 9:25:35 AM
Data Acquisition Time : 6/13/2019 9:21:10 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-002.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

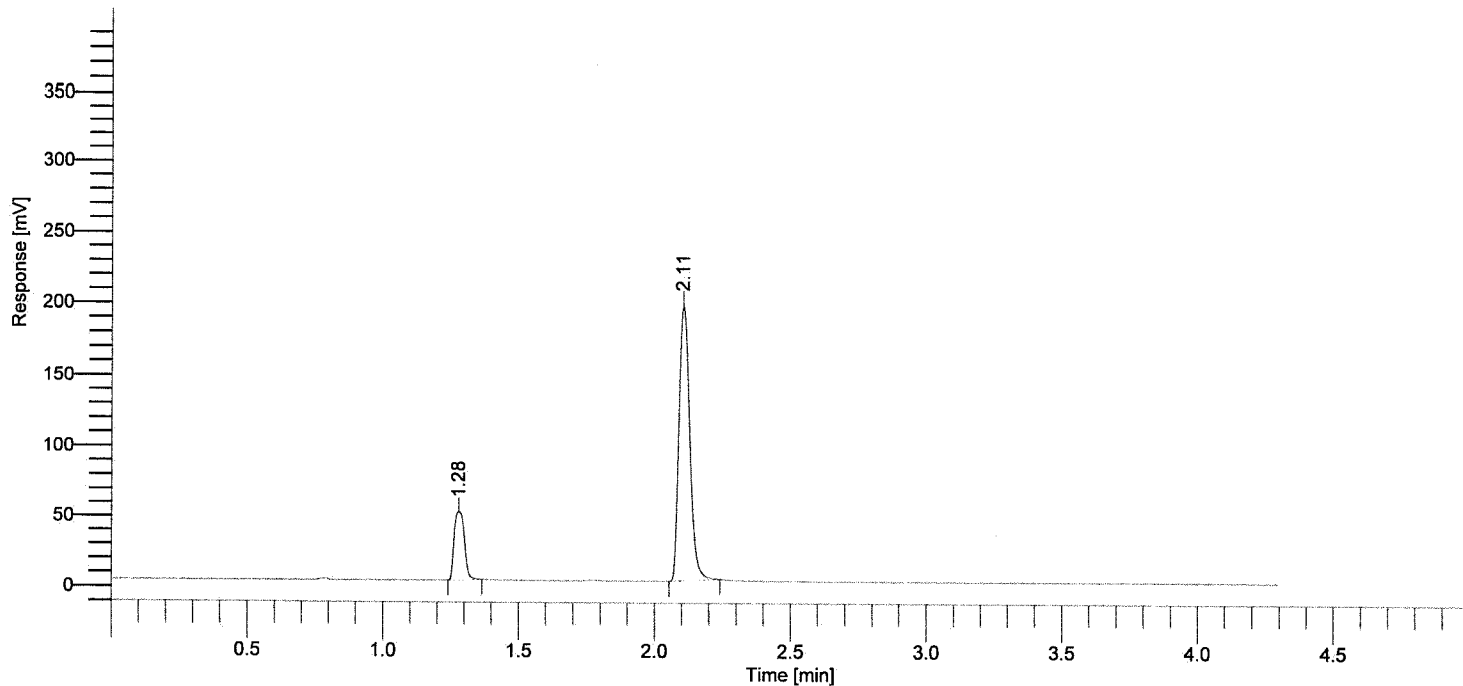

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.0792	1.28	124624.7
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.11	539744.9

6/13/19

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53454
Sample Name : 0.08% CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 2

Date : 6/13/2019 9:25:37 AM
Data Acquisition Time : 6/13/2019 9:21:10 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-002.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

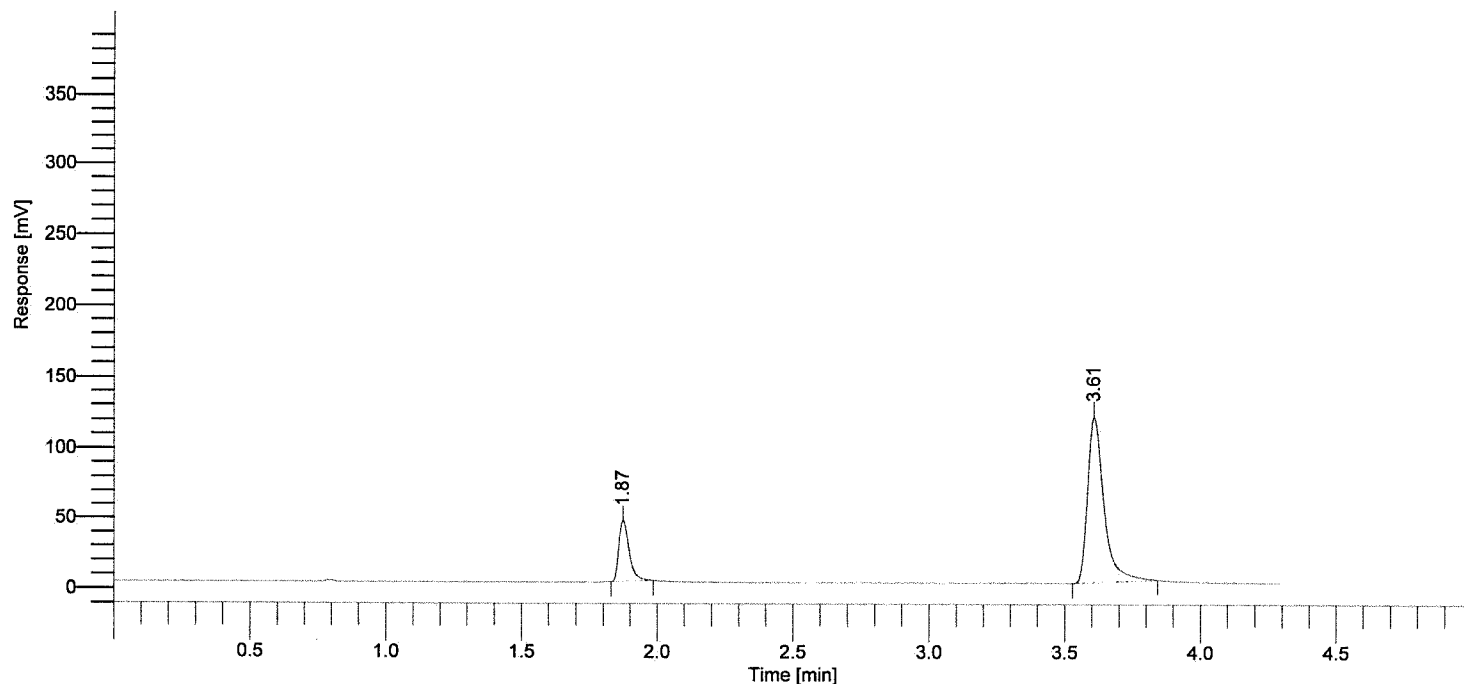

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.61

7ca

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53455
Sample Name : 0.10% CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 3

Date : 6/13/2019 9:30:35 AM
Data Acquisition Time : 6/13/2019 9:26:10 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-003.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

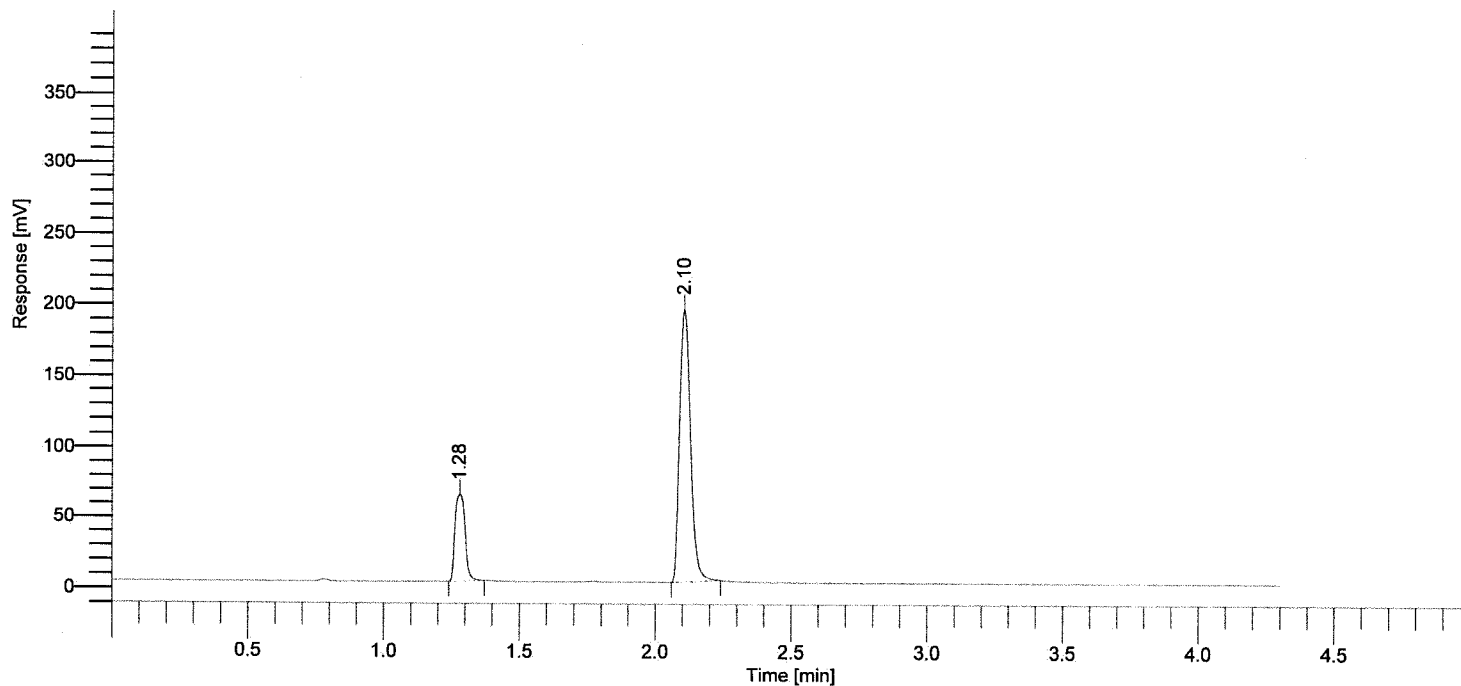

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.0991	1.28	157410.4
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.10	539336.2

8 

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53456
Sample Name : 0.10% CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 3

Date : 6/13/2019 9:30:37 AM
Data Acquisition Time : 6/13/2019 9:26:10 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-003.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

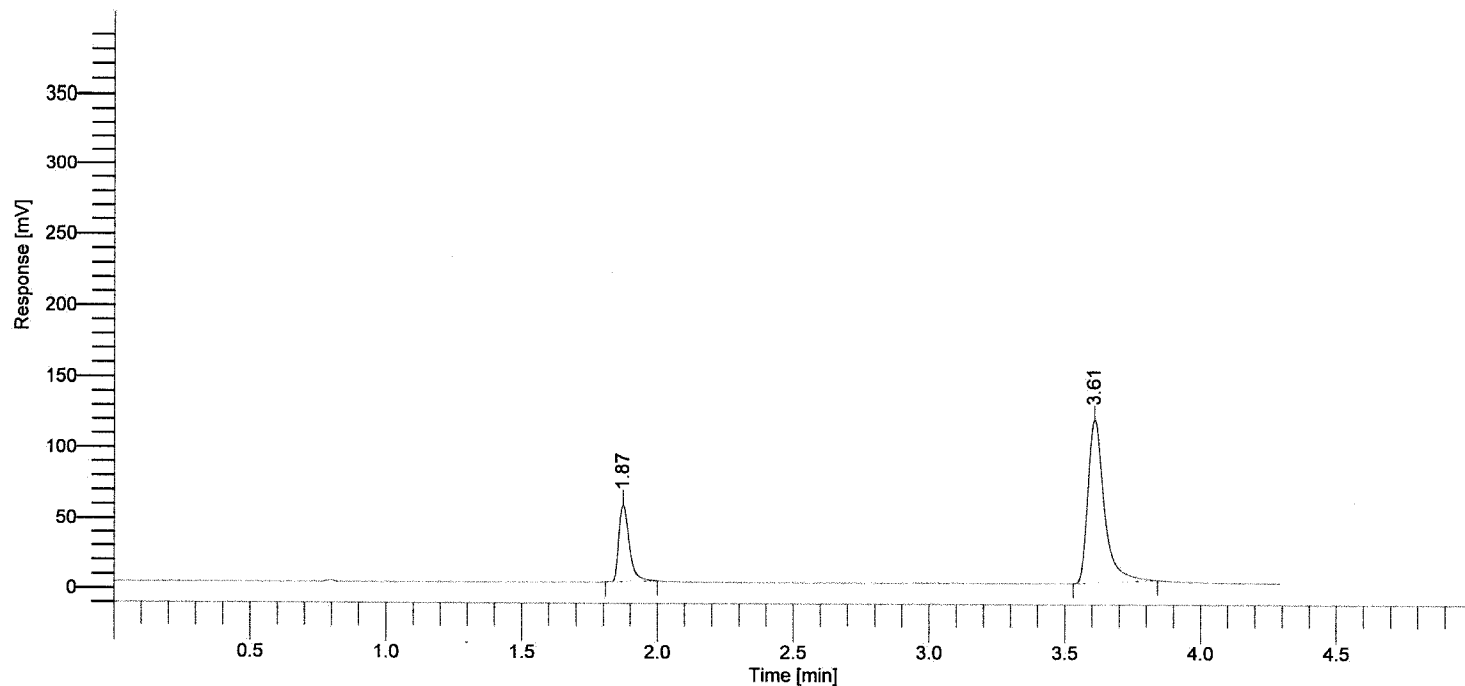

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.61

96

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53457
Sample Name : NEG CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 4

Date : 6/13/2019 9:35:35 AM
Data Acquisition Time : 6/13/2019 9:31:10 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-004.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

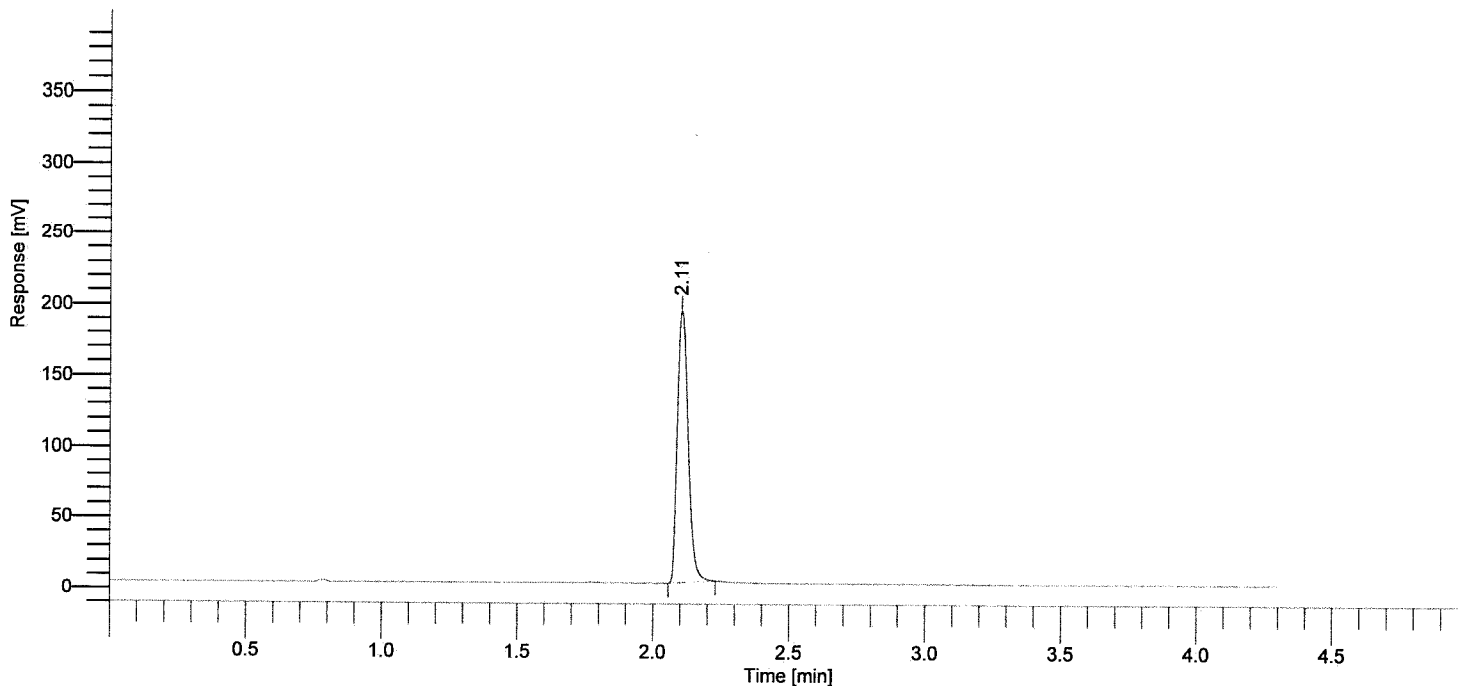

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.0000	1.28	0.0
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.11	534006.8

10 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53458
Sample Name : NEG CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 4

Date : 6/13/2019 9:35:37 AM
Data Acquisition Time : 6/13/2019 9:31:10 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-004.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

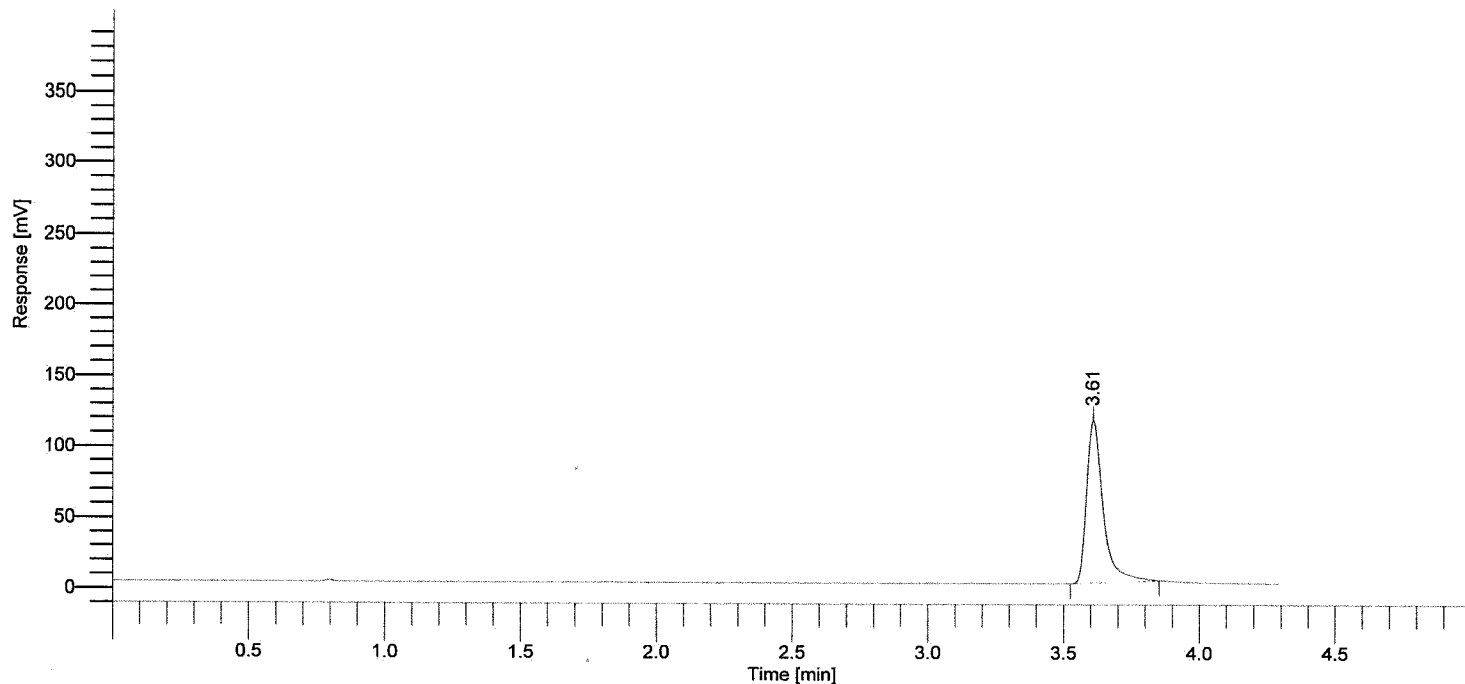

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
N-PROPANOL	3.61

11Cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53459
Sample Name : GUTH 19130 #8
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 5

Date : 6/13/2019 9:40:36 AM
Data Acquisition Time : 6/13/2019 9:36:10 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-005.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

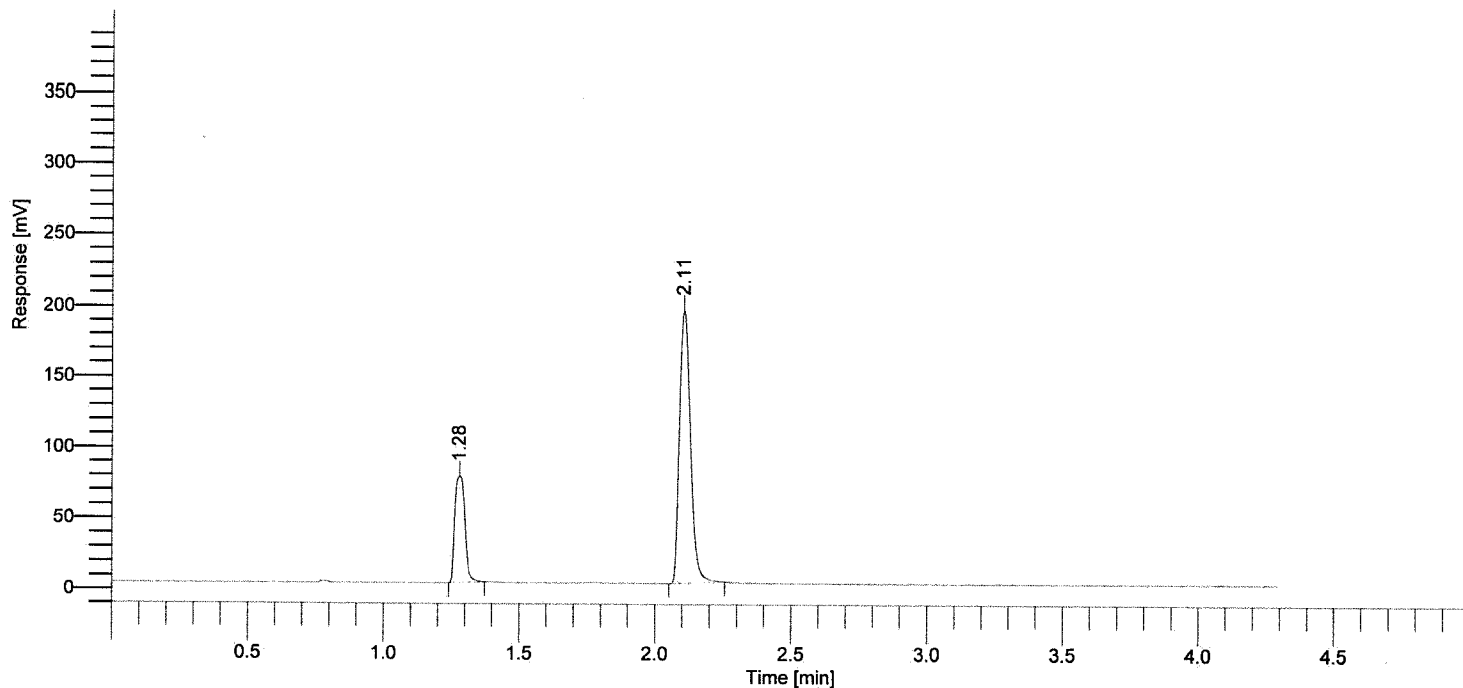

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.1195	1.28	192425.5
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.11	542972.7

12 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53460
Sample Name : GUTH 19130 #8
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 5

Date : 6/13/2019 9:40:37 AM
Data Acquisition Time : 6/13/2019 9:36:10 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-005.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

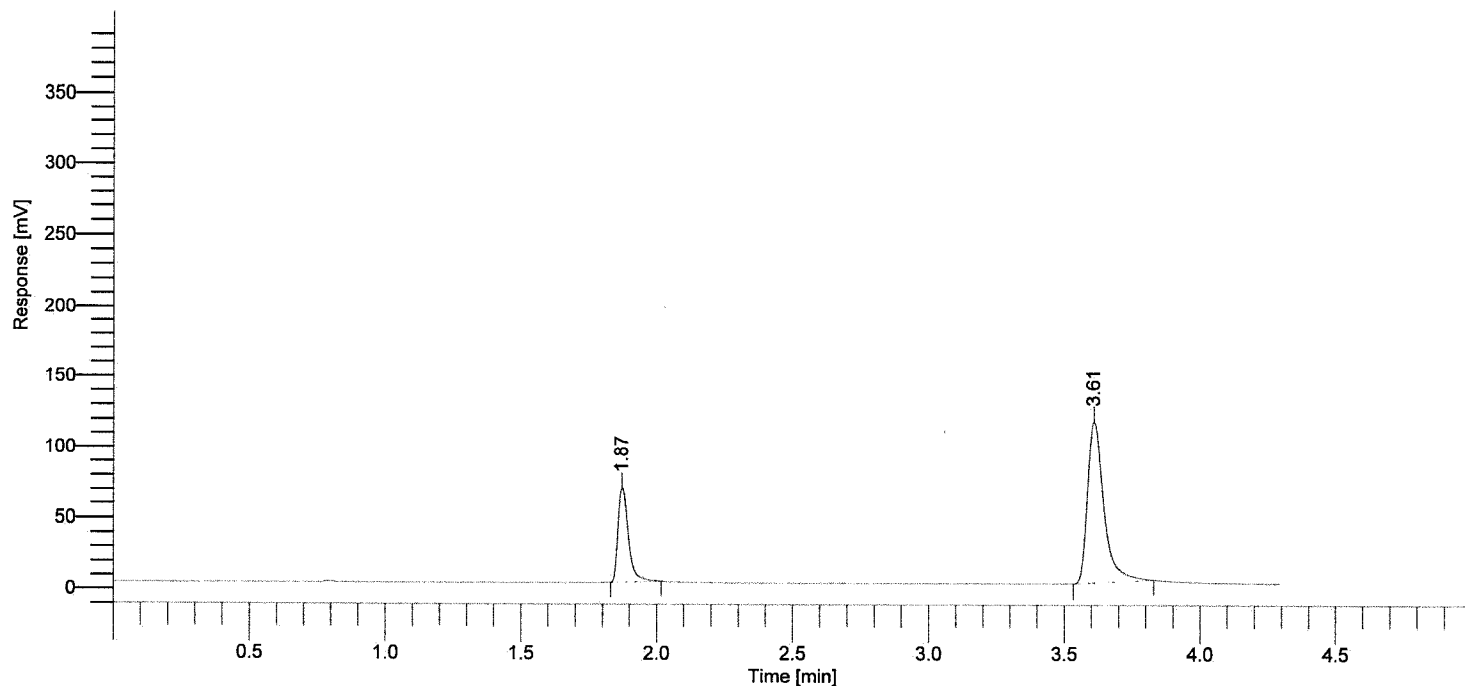

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.61

136

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53461
Sample Name : GUTH 19130 #8
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 6

Date : 6/13/2019 9:45:35 AM
Data Acquisition Time : 6/13/2019 9:41:10 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-006.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

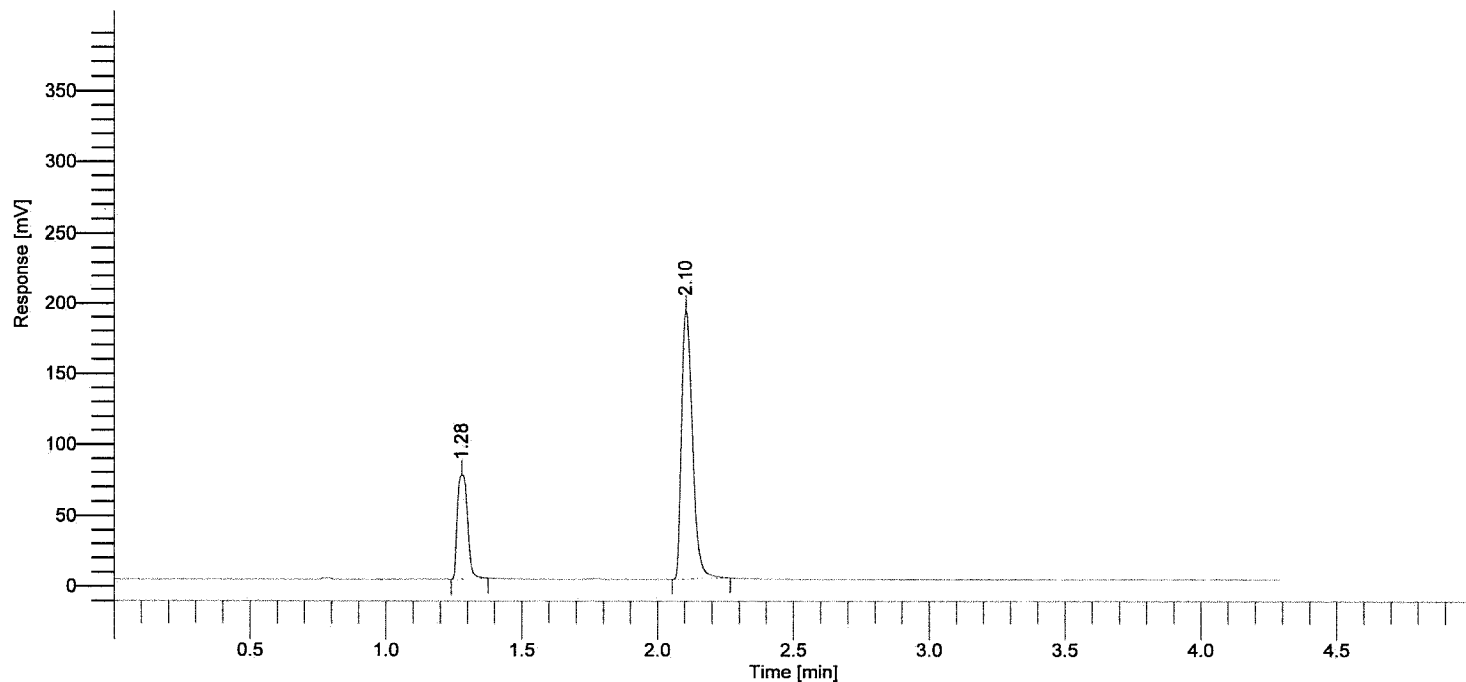

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.1192	1.28	188542.6
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.10	533346.7

1402

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53462
Sample Name : GUTH 19130 #8
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 6

Date : 6/13/2019 9:45:37 AM
Data Acquisition Time : 6/13/2019 9:41:10 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-006.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

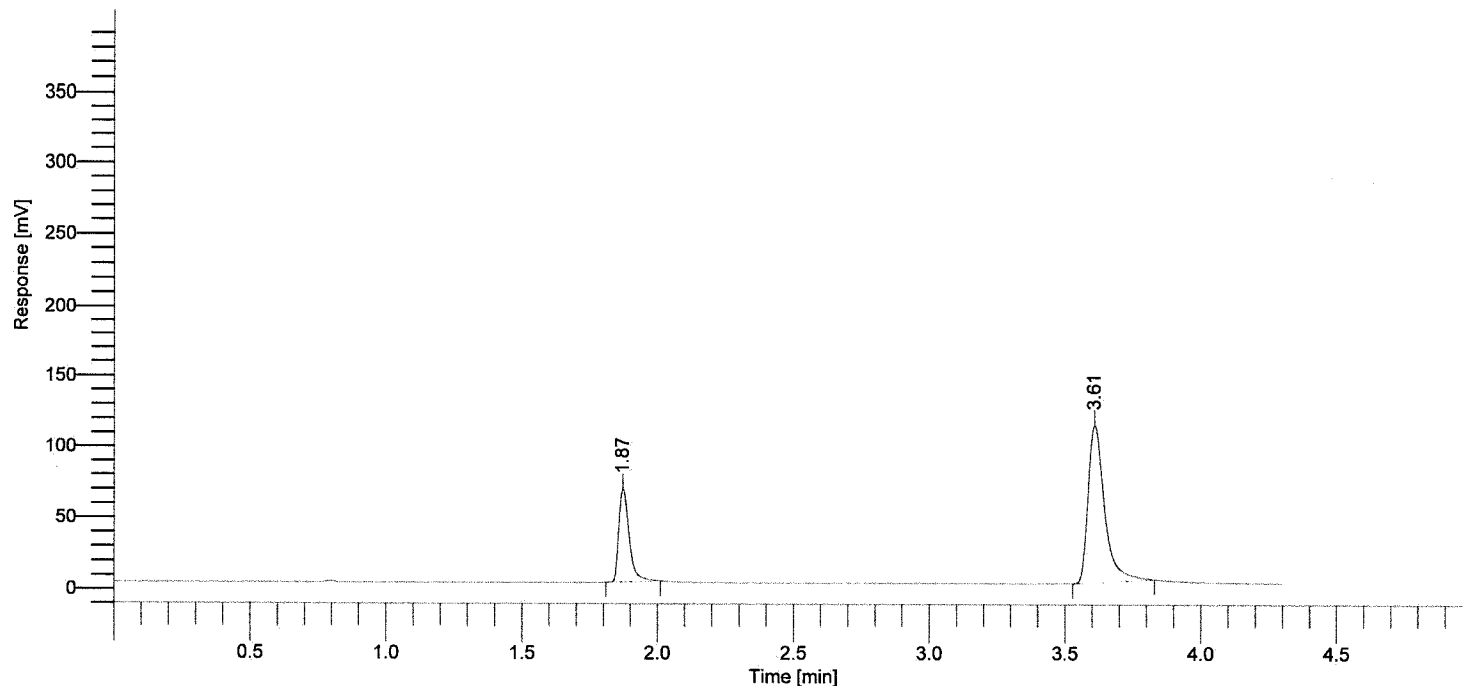

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.61

15 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53463
Sample Name : GUTH 19130 #8
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 7

Date : 6/13/2019 9:50:36 AM
Data Acquisition Time : 6/13/2019 9:46:10 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-007.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

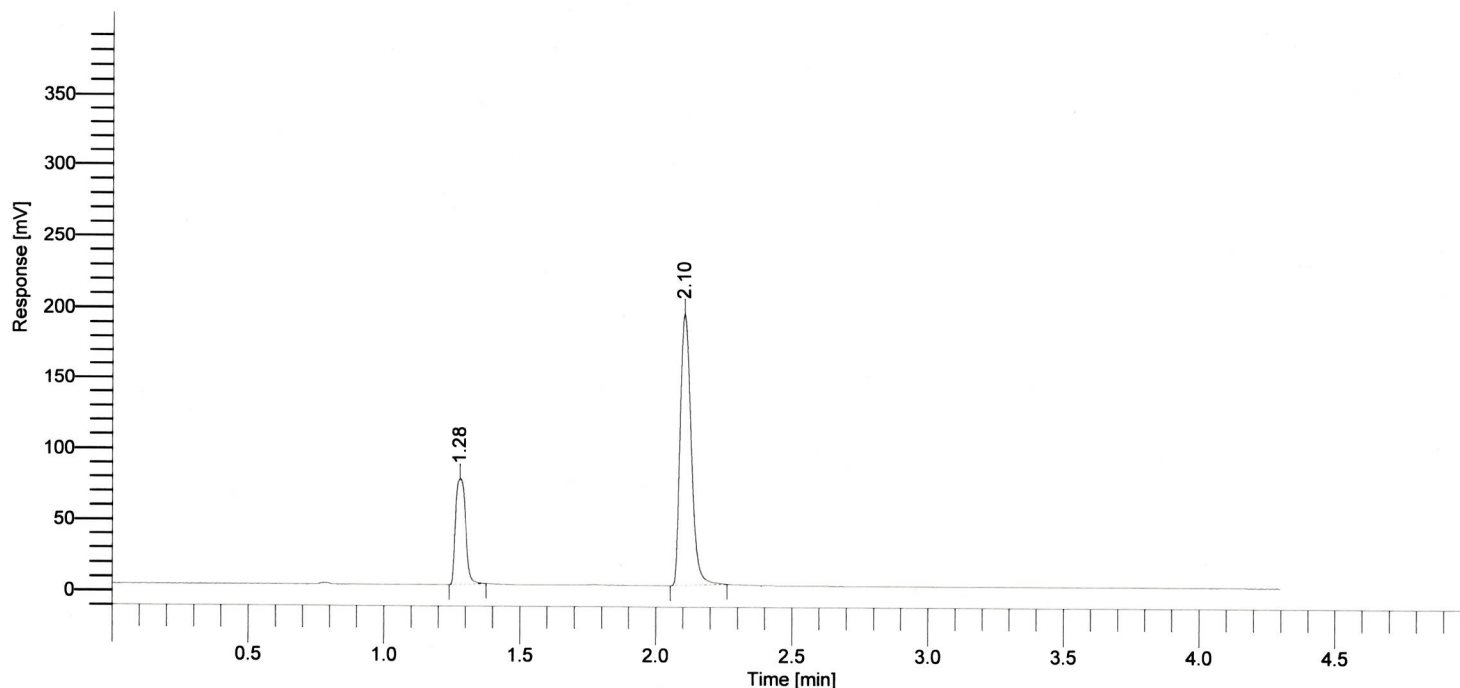

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.1190	1.28	190518.9
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.10	539996.5

Handwritten signature

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53464
Sample Name : GUTH 19130 #8
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 7

Date : 6/13/2019 9:50:37 AM
Data Acquisition Time : 6/13/2019 9:46:10 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-007.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

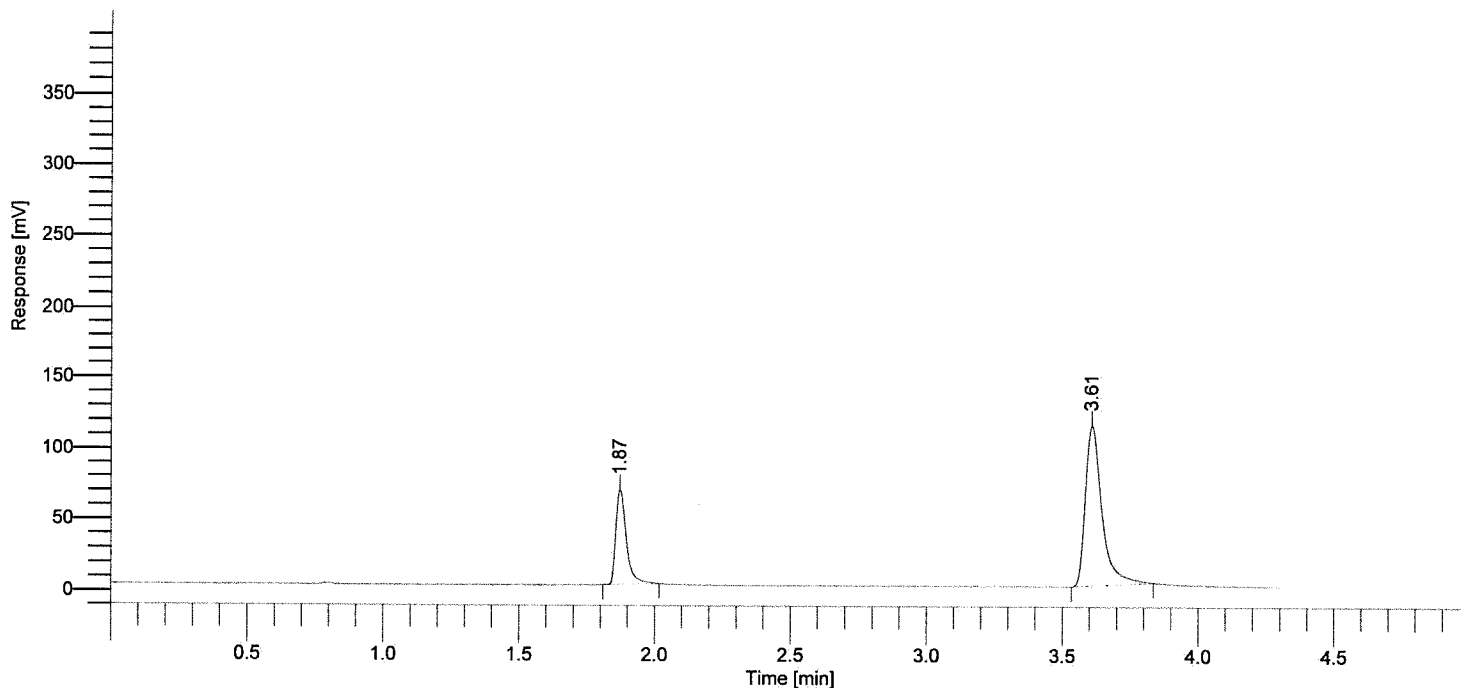

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.61

17cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53465
Sample Name : GUTH 19130 #9
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 8

Date : 6/13/2019 9:55:35 AM
Data Acquisition Time : 6/13/2019 9:51:10 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-008.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

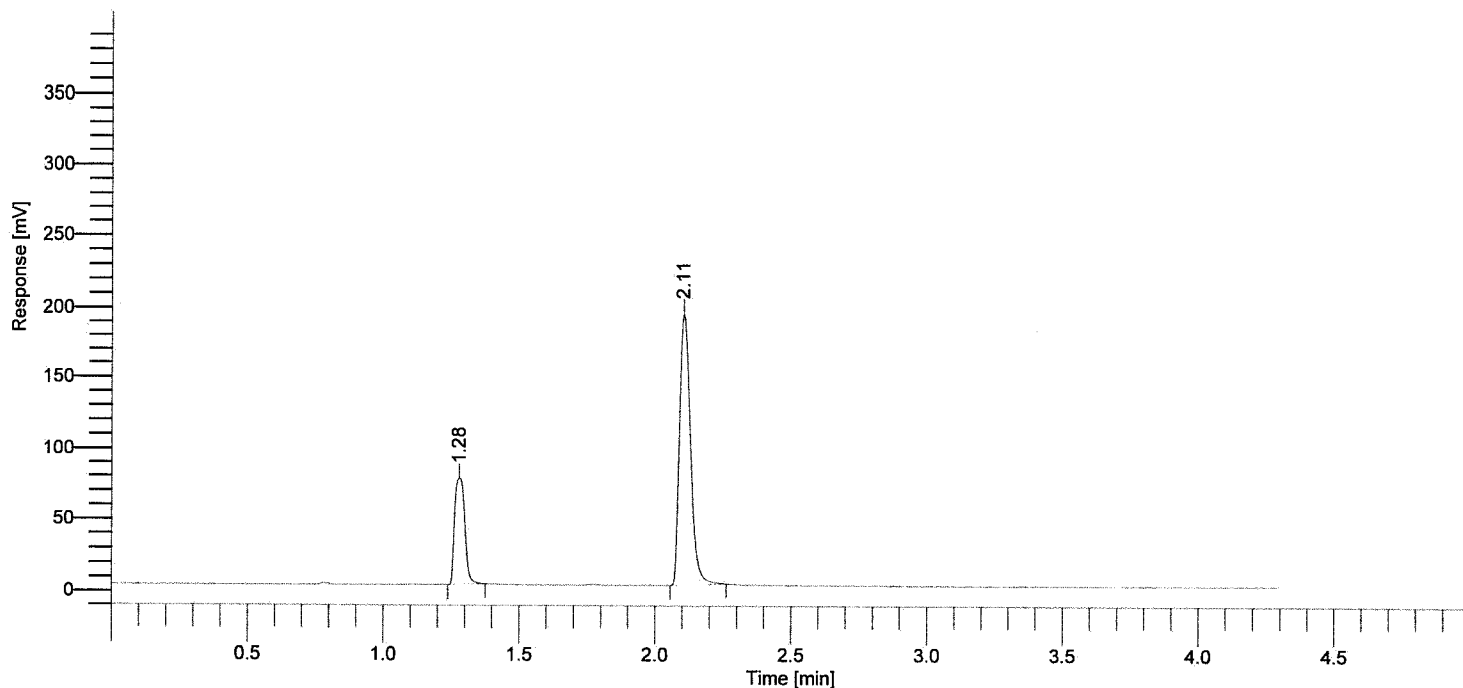

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.1191	1.28	189926.8
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.11	537585.1

18 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53466
Sample Name : GUTH 19130 #9
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 8

Date : 6/13/2019 9:55:37 AM
Data Acquisition Time : 6/13/2019 9:51:10 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-008.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

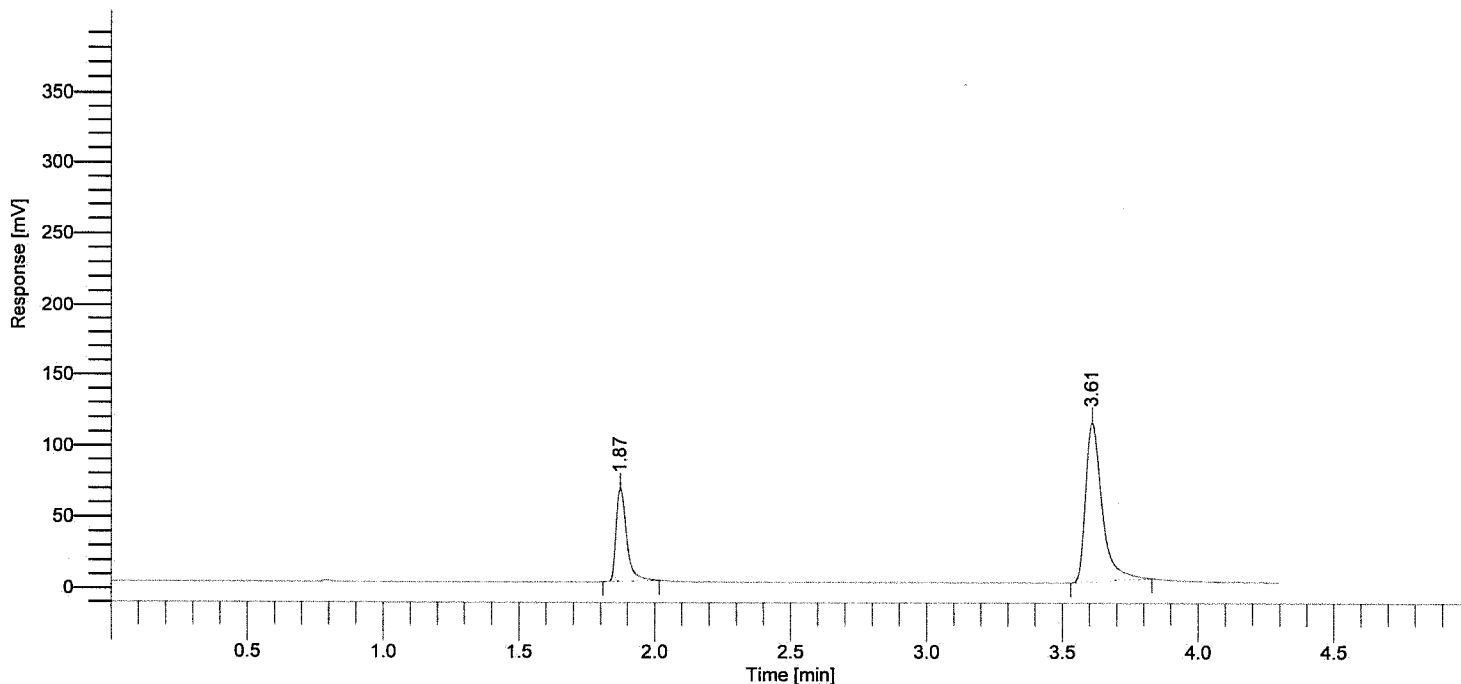

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.61

19 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53467
Sample Name : GUTH 19130 #9
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 9

Date : 6/13/2019 10:00:35 AM
Data Acquisition Time : 6/13/2019 9:56:10 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-009.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

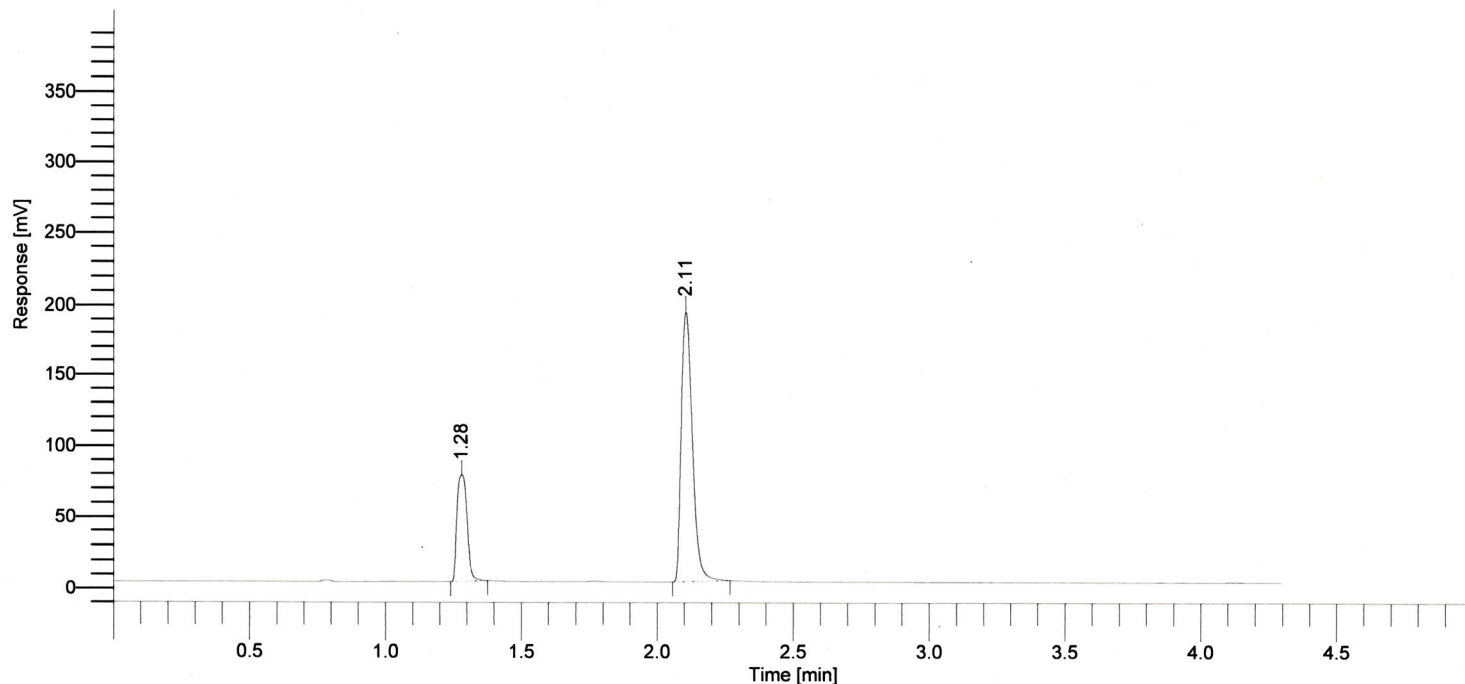

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.1189	1.28	190340.8
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.11	539649.7

20 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53468
Sample Name : GUTH 19130 #9
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 9

Date : 6/13/2019 10:00:37 AM
Data Acquisition Time : 6/13/2019 9:56:10 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-009.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

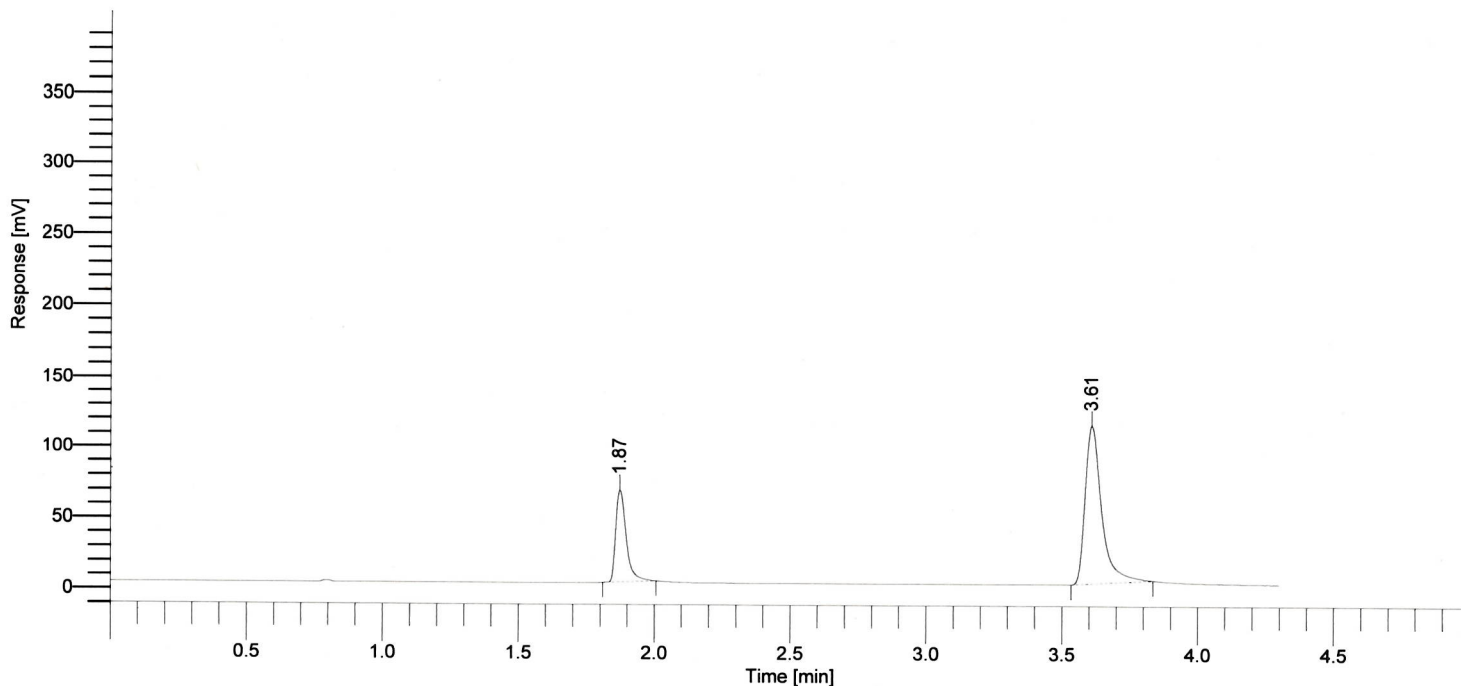

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.61

21 Can

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53469
Sample Name : GUTH 19130 #9
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 10

Date : 6/13/2019 10:05:36 AM
Data Acquisition Time : 6/13/2019 10:01:10 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-010.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

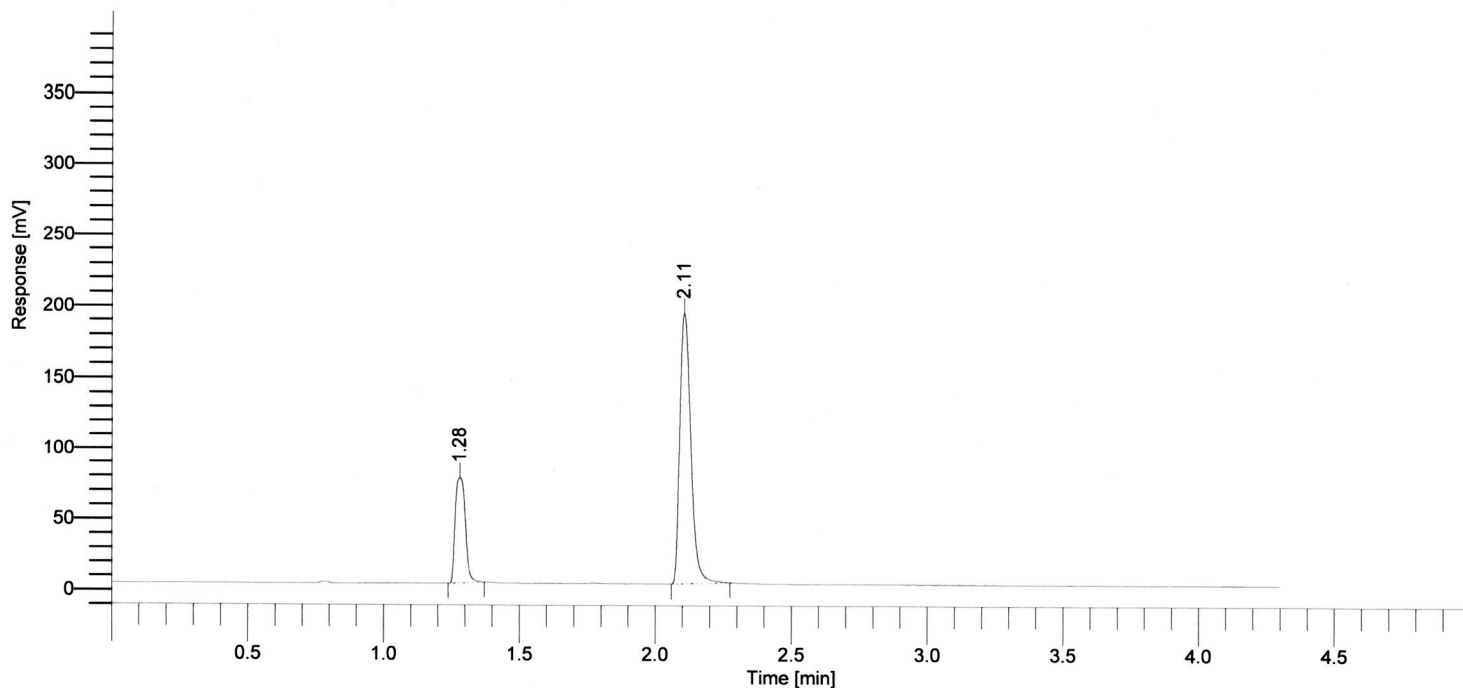

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.1183	1.28	190000.8
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.11	541415.4

22 Cam

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53470
Sample Name : GUTH 19130 #9
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 10

Date : 6/13/2019 10:05:37 AM
Data Acquisition Time : 6/13/2019 10:01:10 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-010.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

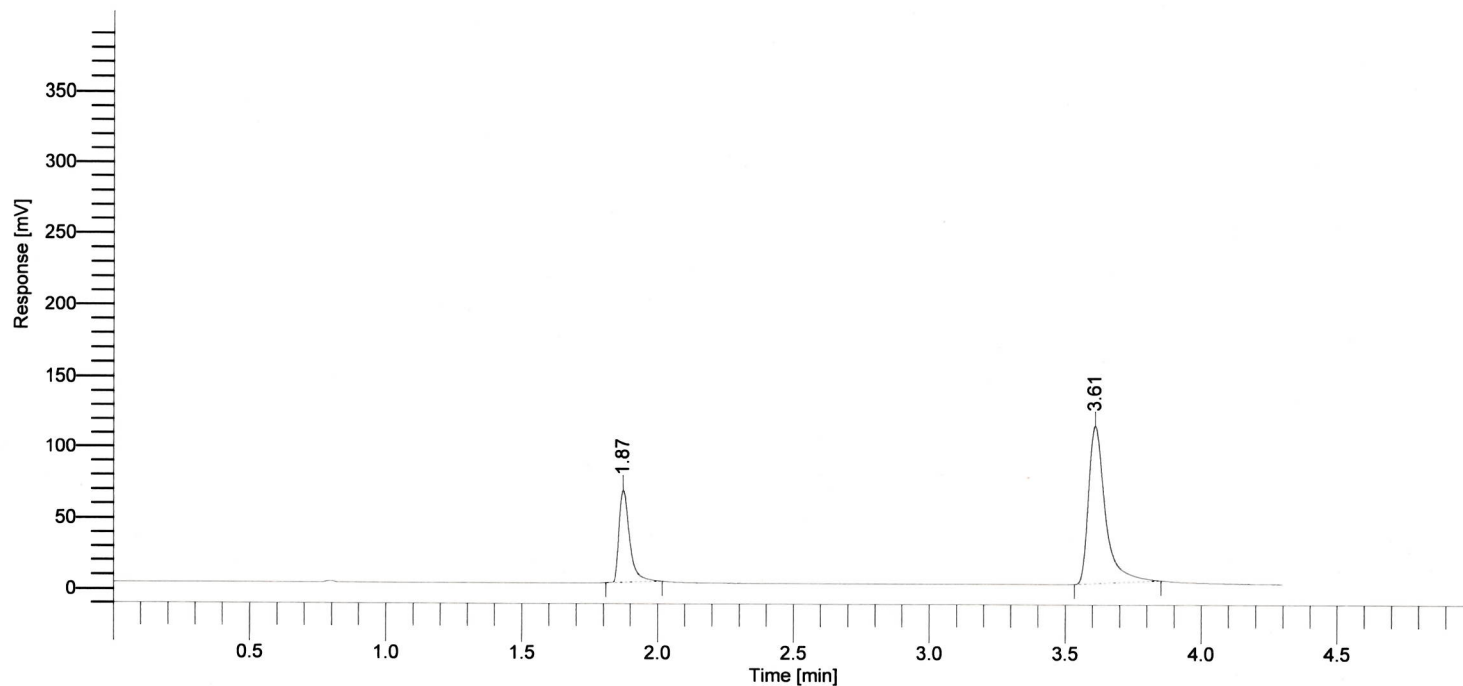

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.61

23 Cam

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53471
Sample Name : GUTH 19130 #732
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 11

Date : 6/13/2019 10:10:36 AM
Data Acquisition Time : 6/13/2019 10:06:10 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-011.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

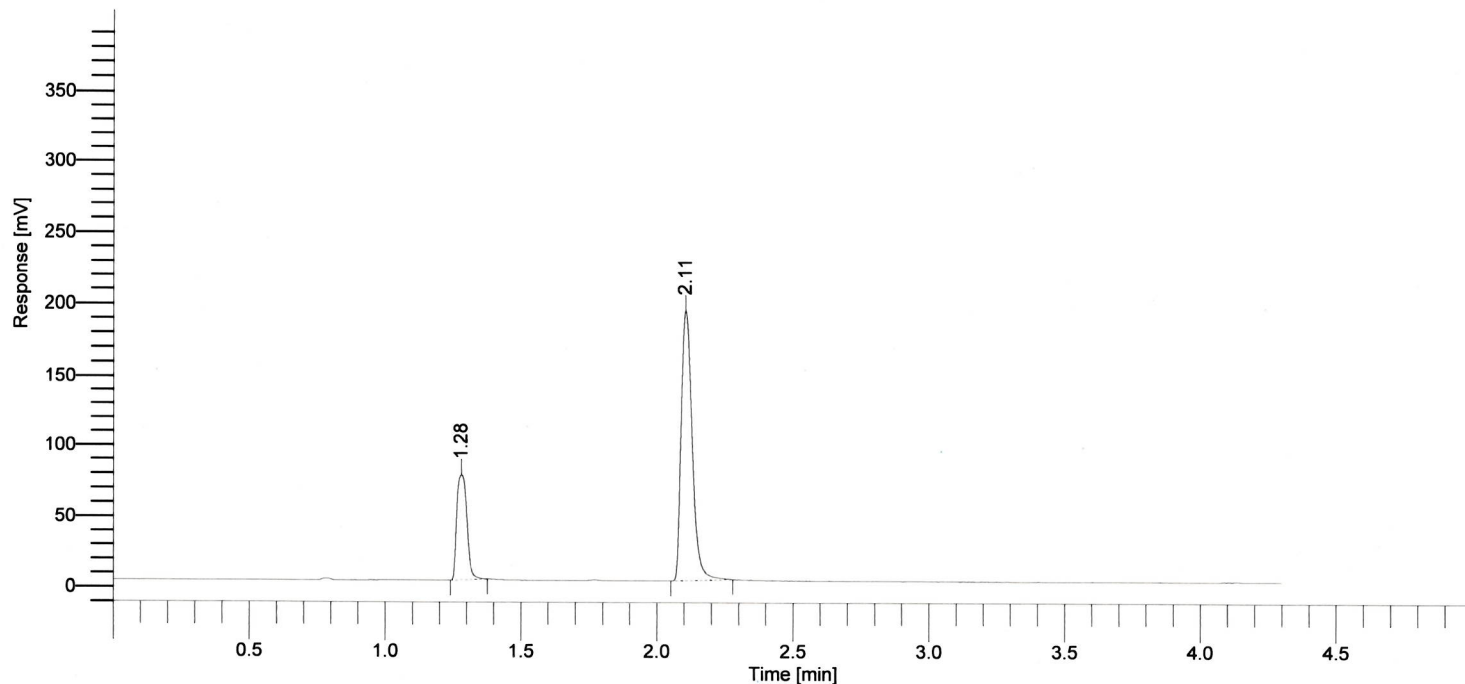

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.1189	1.28	190467.7
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.11	539966.8

24 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53472
Sample Name : GUTH 19130 #732
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 11

Date : 6/13/2019 10:10:37 AM
Data Acquisition Time : 6/13/2019 10:06:10 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-011.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

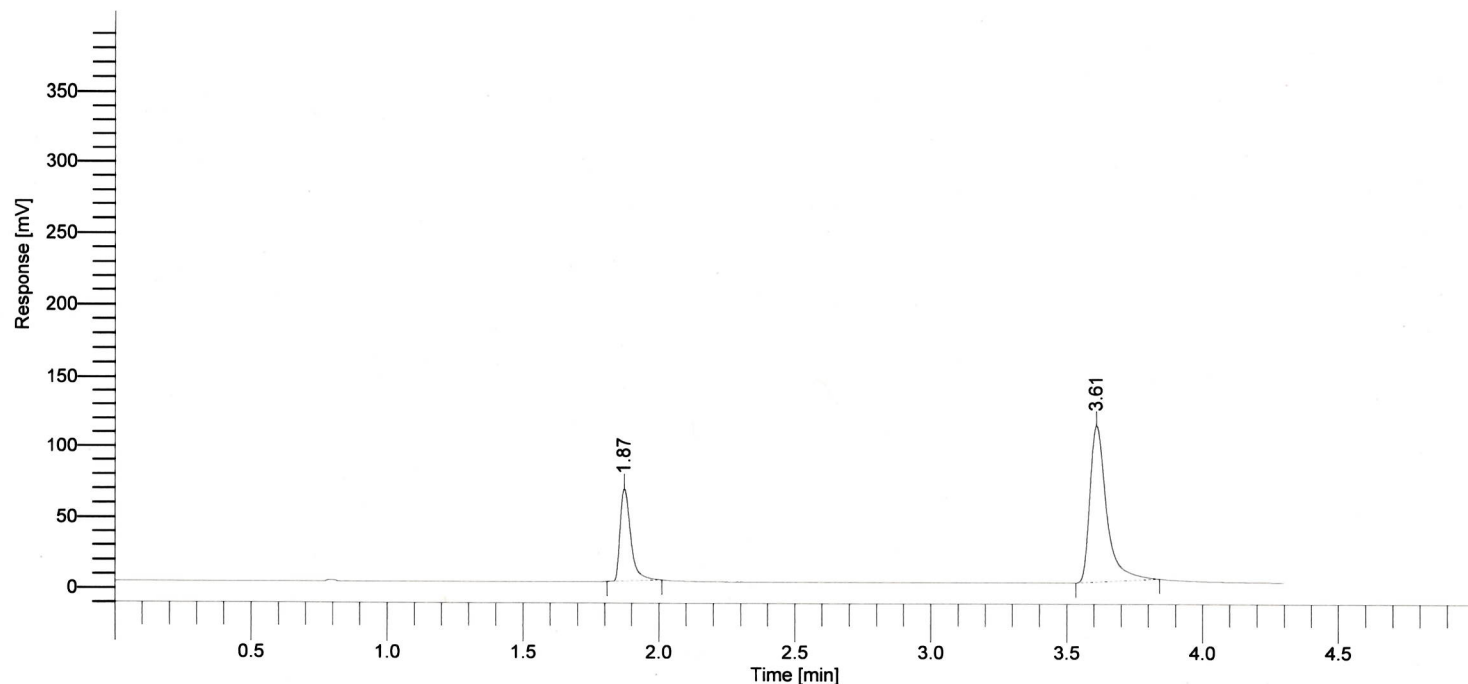

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.61

25 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53473
Sample Name : GUTH 19130 #732
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 12

Date : 6/13/2019 10:15:36 AM
Data Acquisition Time : 6/13/2019 10:11:10 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-012.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

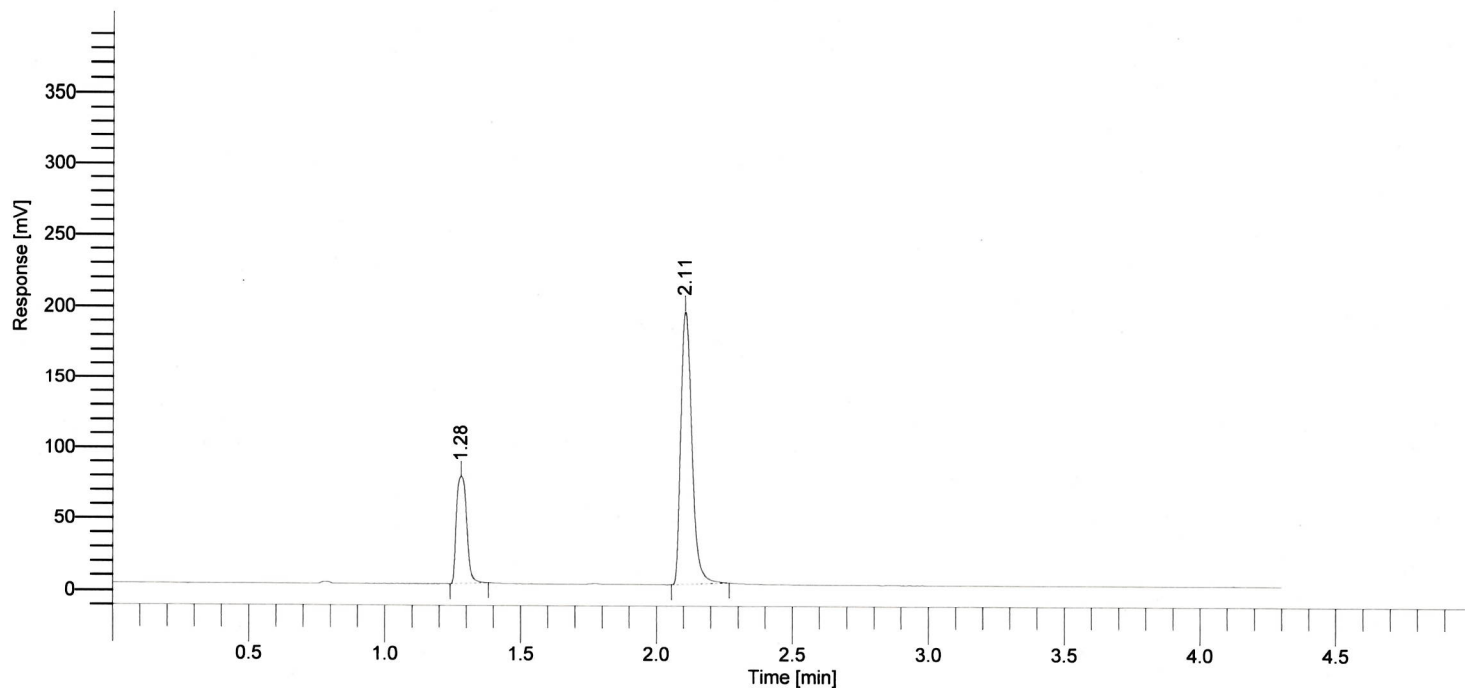

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.1195	1.28	193321.0
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.11	545536.9

26 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53474
Sample Name : GUTH 19130 #732
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 12

Date : 6/13/2019 10:15:37 AM
Data Acquisition Time : 6/13/2019 10:11:10 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-012.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

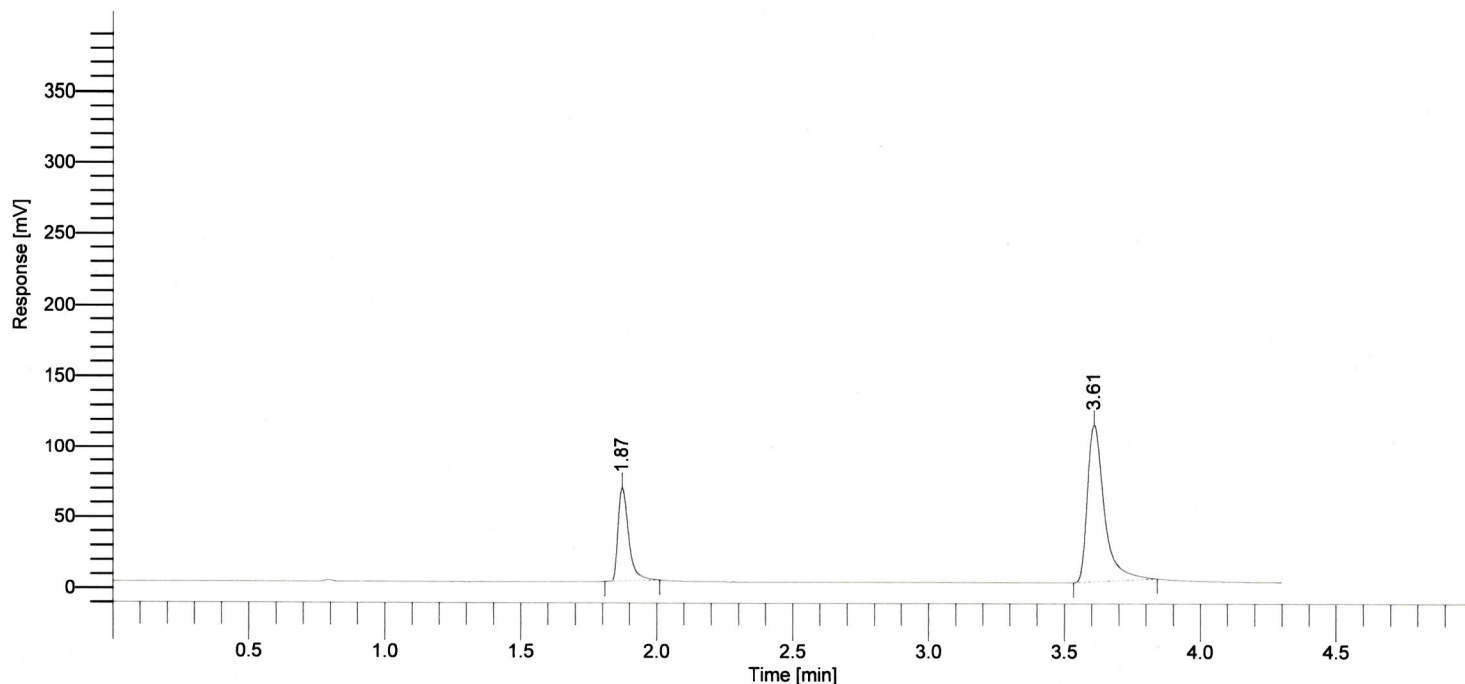

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.61

27

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53475
Sample Name : GUTH 19130 #732
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 13

Date : 6/13/2019 10:20:36 AM
Data Acquisition Time : 6/13/2019 10:16:10 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-013.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

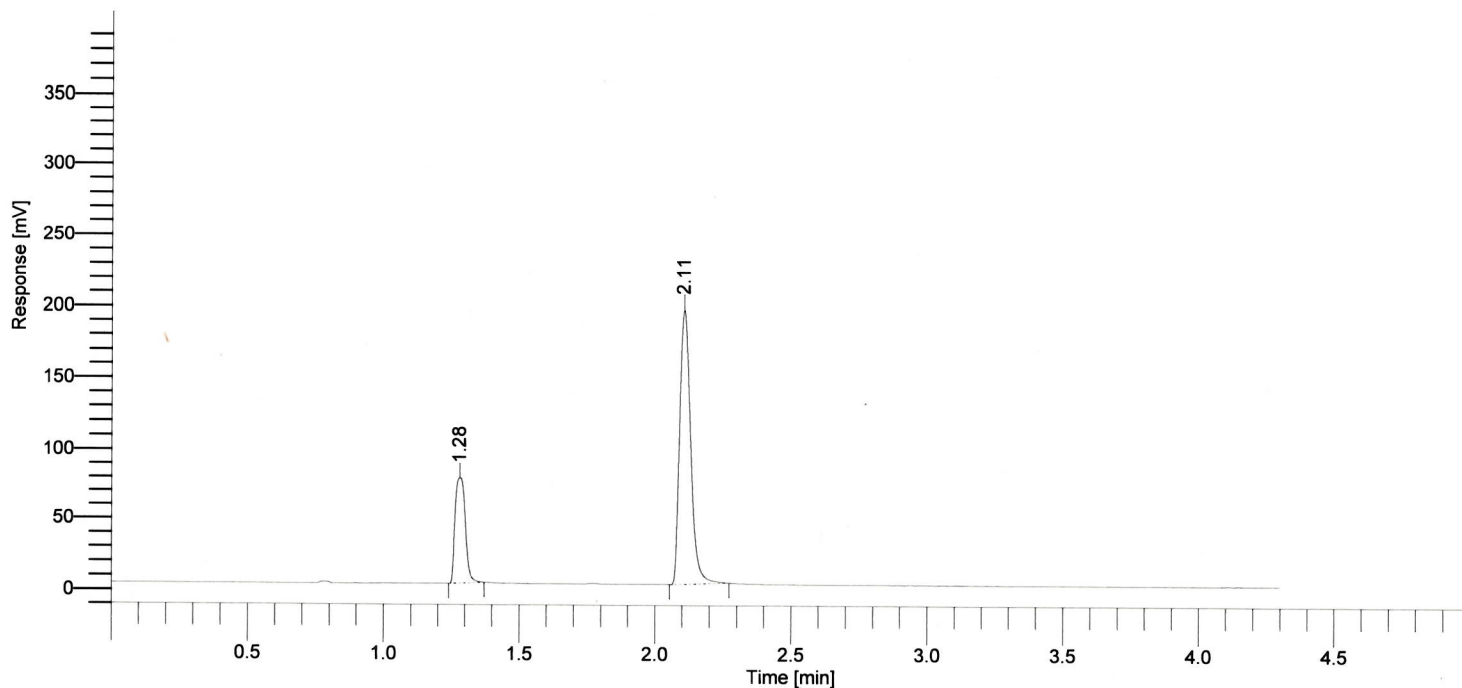

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.1189	1.28	192733.7
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.11	546690.6

28 Cam

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53476
Sample Name : GUTH 19130 #732
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 13

Date : 6/13/2019 10:20:37 AM
Data Acquisition Time : 6/13/2019 10:16:10 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-013.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

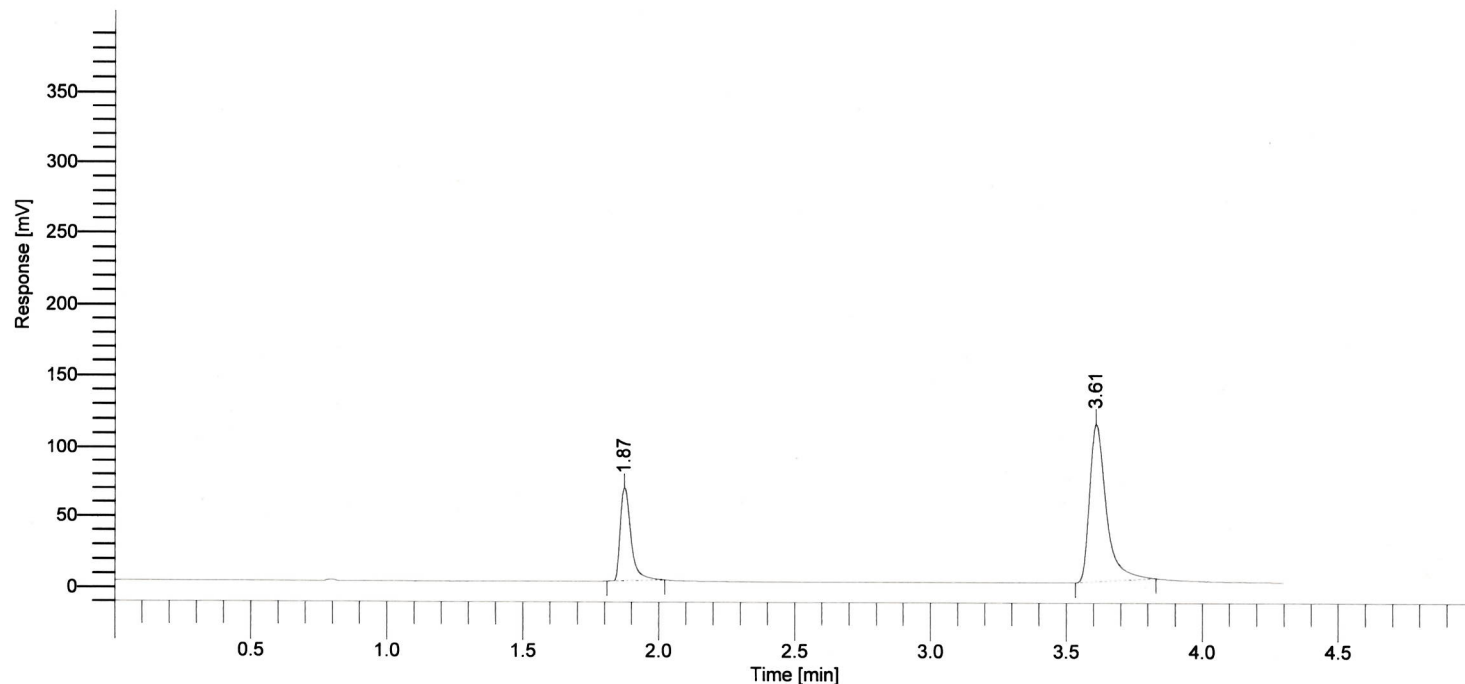

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.61

Handwritten signature

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53477
Sample Name : 0.10% CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 14

Date : 6/13/2019 10:25:36 AM
Data Acquisition Time : 6/13/2019 10:21:10 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-014.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

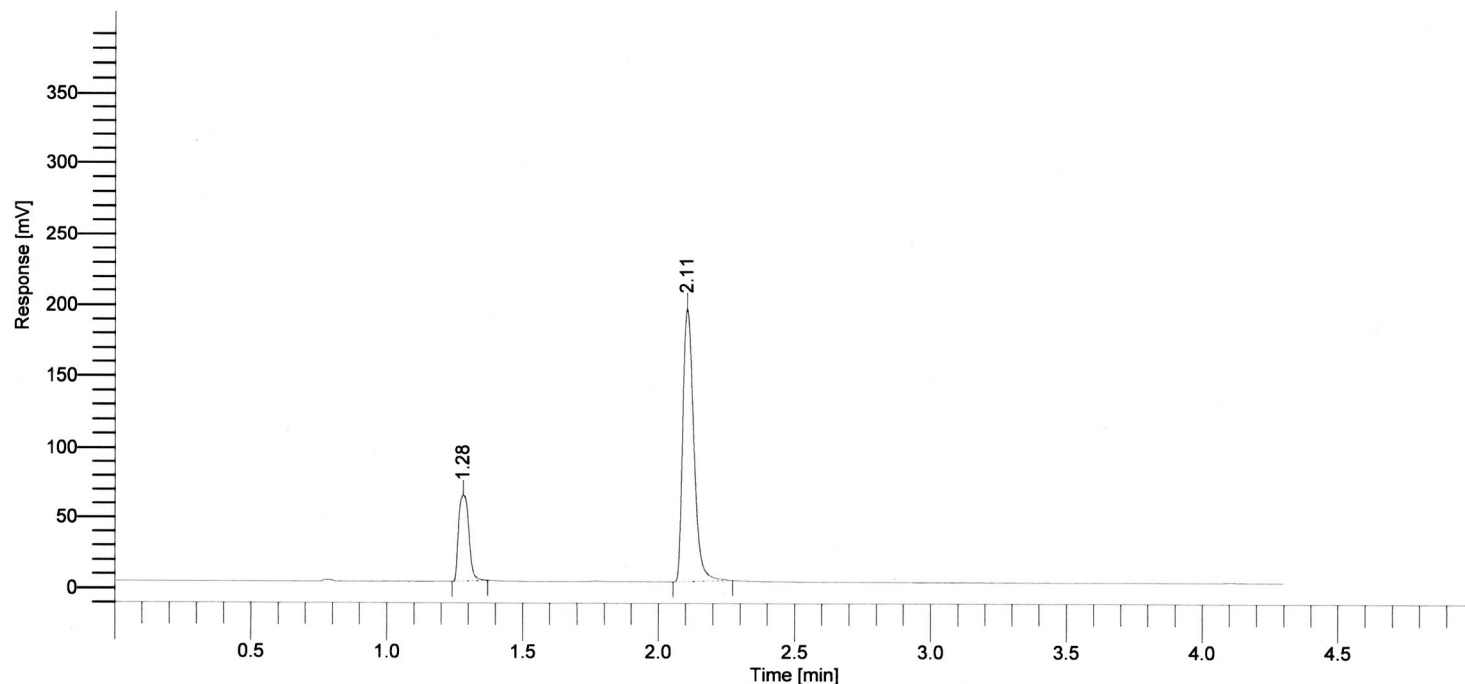

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.0980	1.28	157129.1
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.11	544667.2

30 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53478
Sample Name : 0.10% CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 14

Date : 6/13/2019 10:25:37 AM
Data Acquisition Time : 6/13/2019 10:21:10 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-014.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

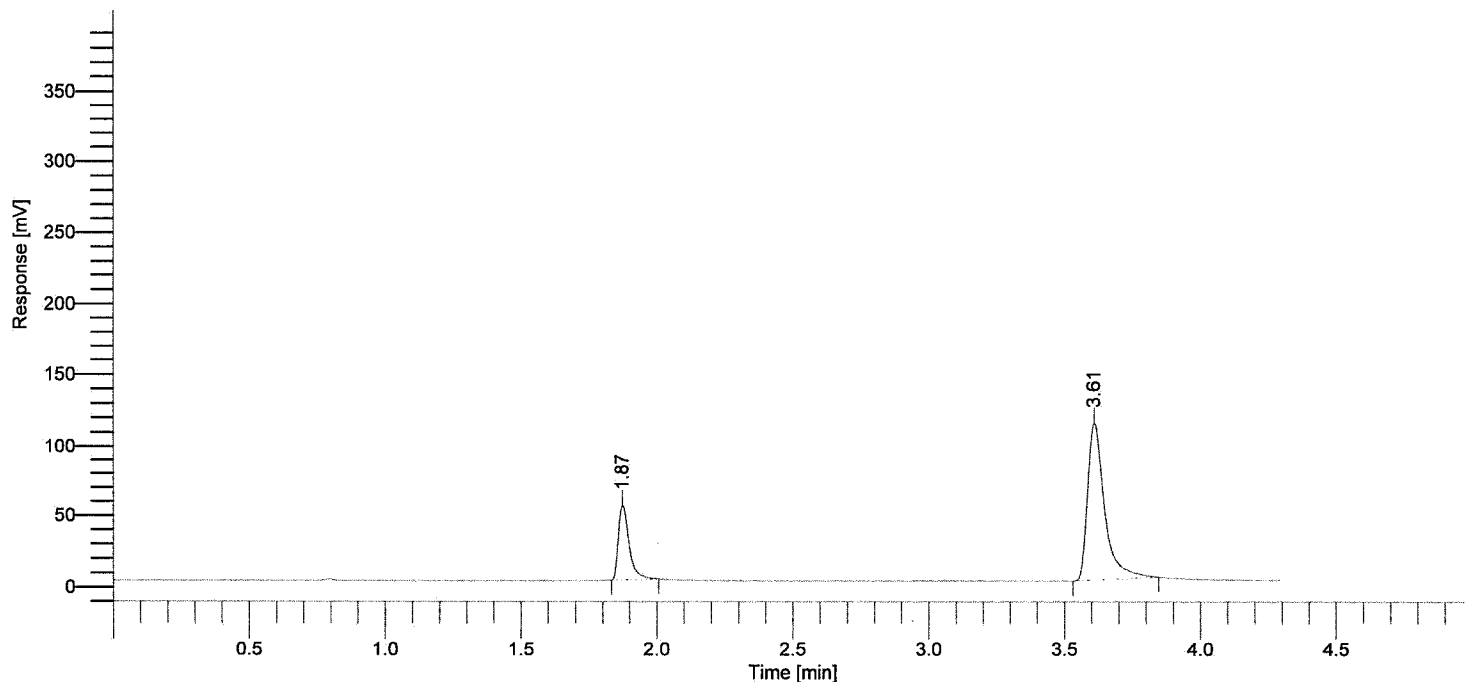

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.61

31 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53479
Sample Name : NEG CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 15

Date : 6/13/2019 10:30:36 AM
Data Acquisition Time : 6/13/2019 10:26:11 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-015.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

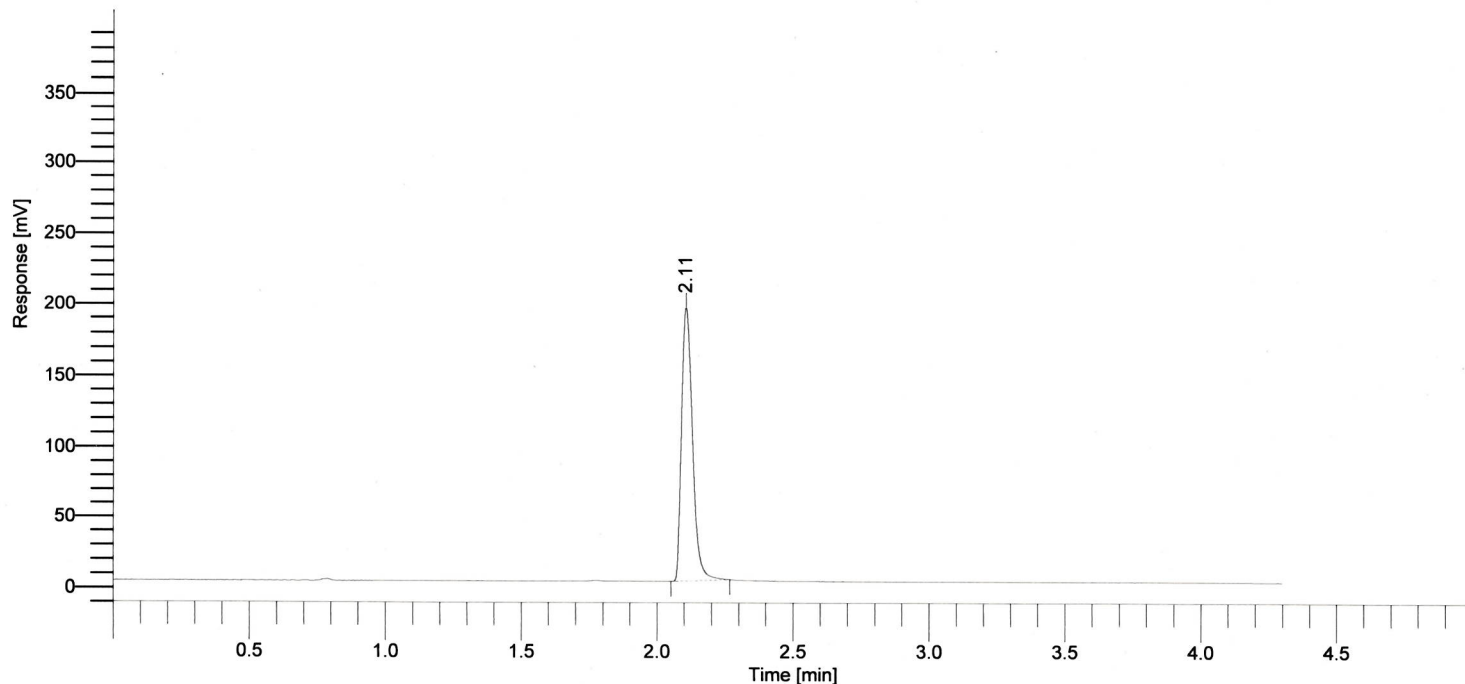

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.0000	1.28	0.0
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.11	543939.0

32 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53480
Sample Name : NEG CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 15

Date : 6/13/2019 10:30:37 AM
Data Acquisition Time : 6/13/2019 10:26:11 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-015.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

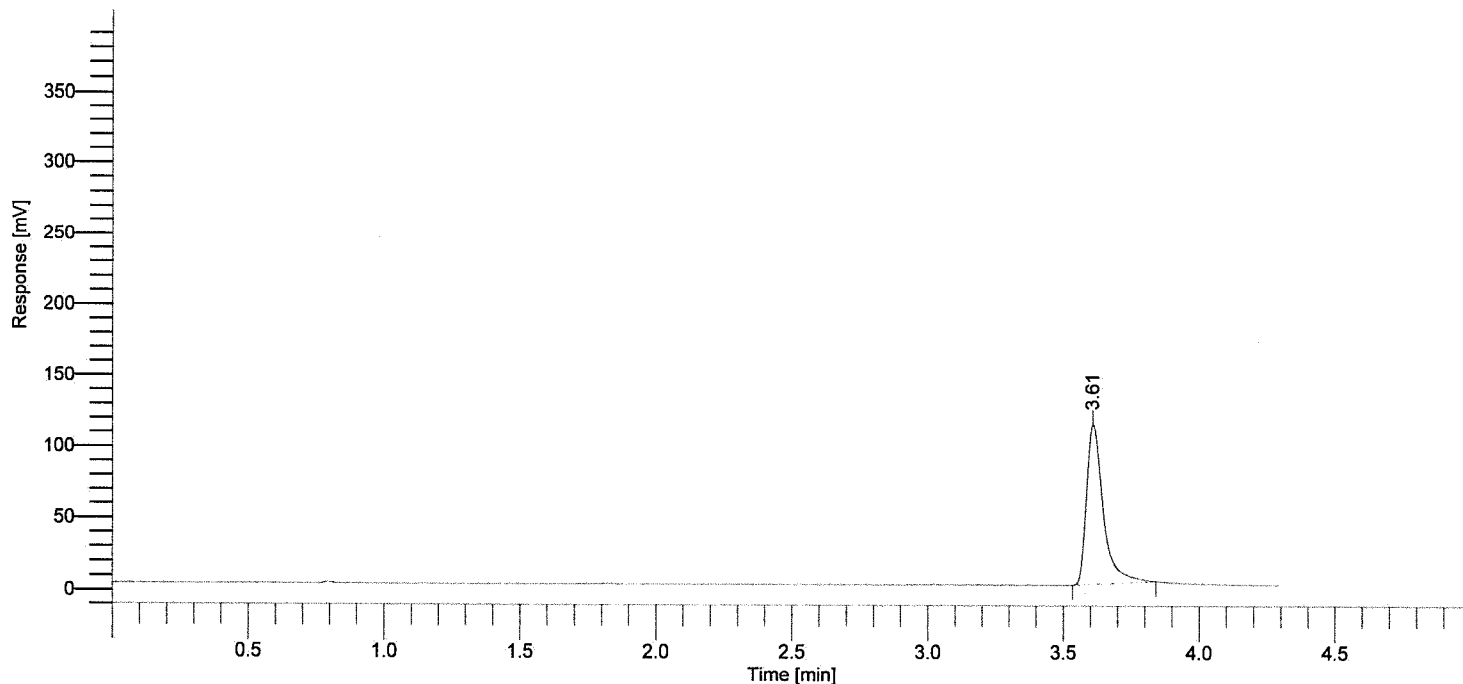

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
N-PROPANOL	3.61

330

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53481
Sample Name : GUTH 19130 #733
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 16

Date : 6/13/2019 10:35:36 AM
Data Acquisition Time : 6/13/2019 10:31:11 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-016.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

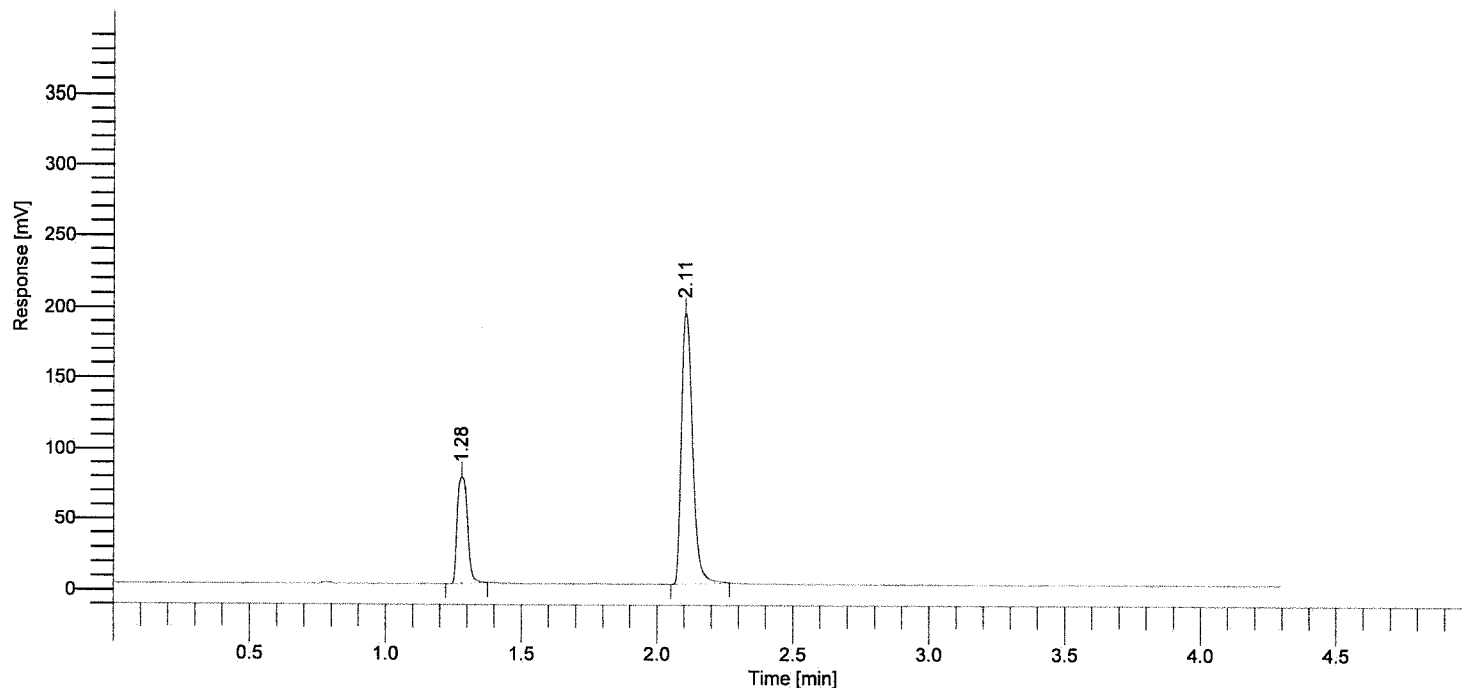

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.1193	1.28	192920.8
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.11	545227.6

34

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53482
Sample Name : GUTH 19130 #733
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 16

Date : 6/13/2019 10:35:37 AM
Data Acquisition Time : 6/13/2019 10:31:11 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-016.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

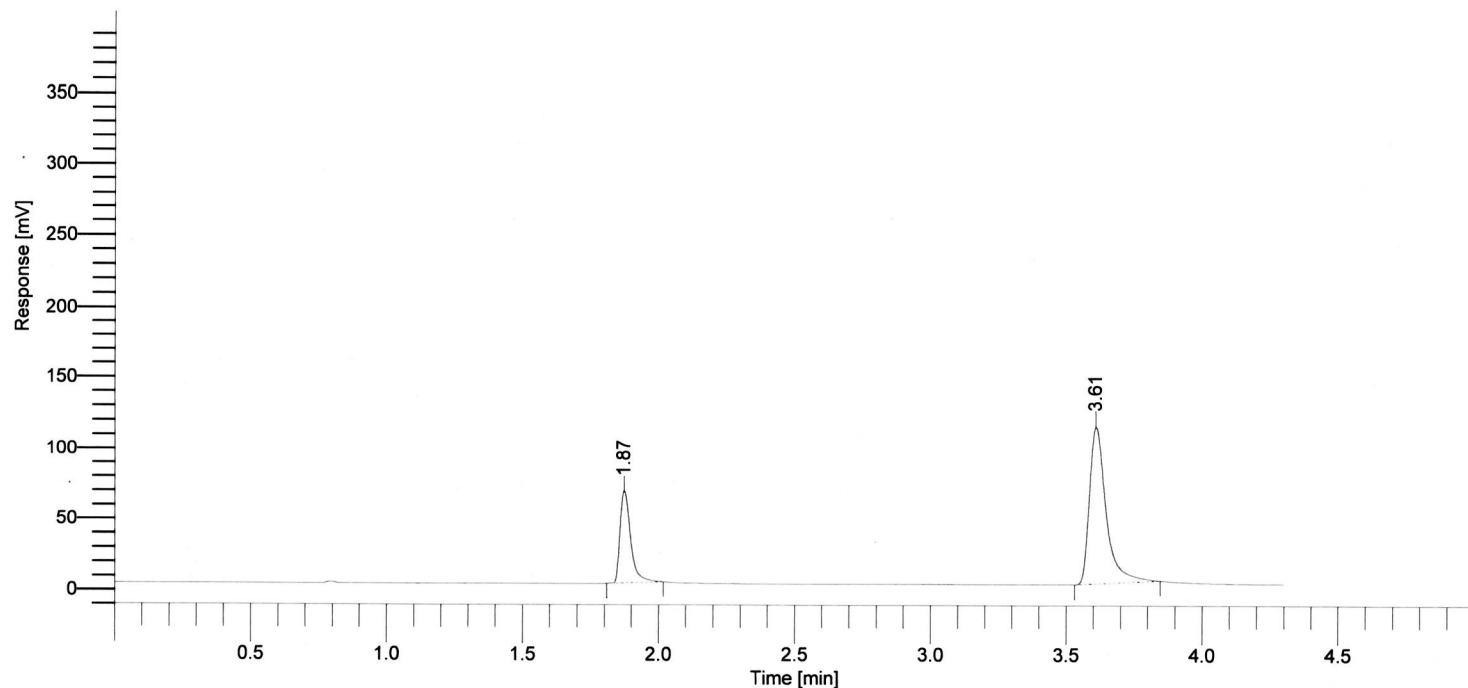

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.61

35 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53483
Sample Name : GUTH 19130 #733
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 17

Date : 6/13/2019 10:40:35 AM
Data Acquisition Time : 6/13/2019 10:36:11 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-017.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

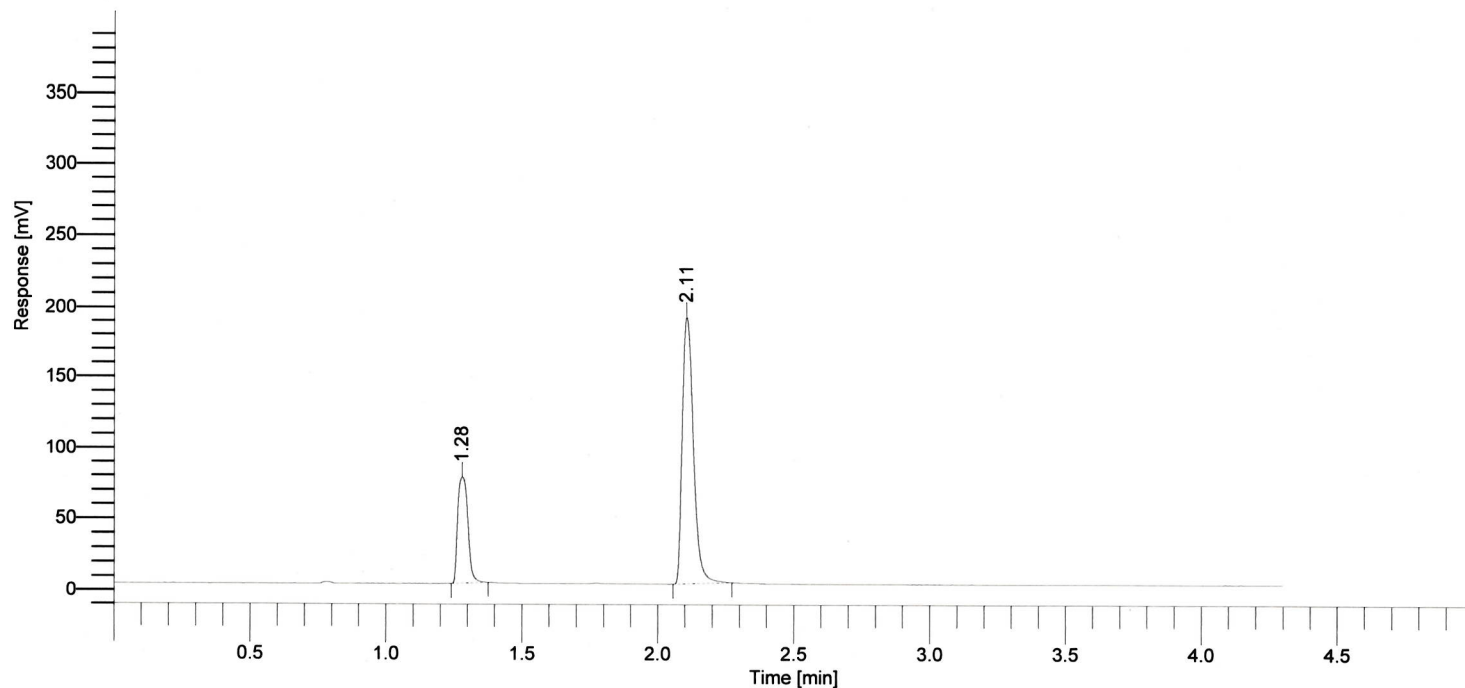

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.1194	1.28	190465.2
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.11	537528.4

366

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53484
Sample Name : GUTH 19130 #733
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 17

Date : 6/13/2019 10:40:37 AM
Data Acquisition Time : 6/13/2019 10:36:11 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-017.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

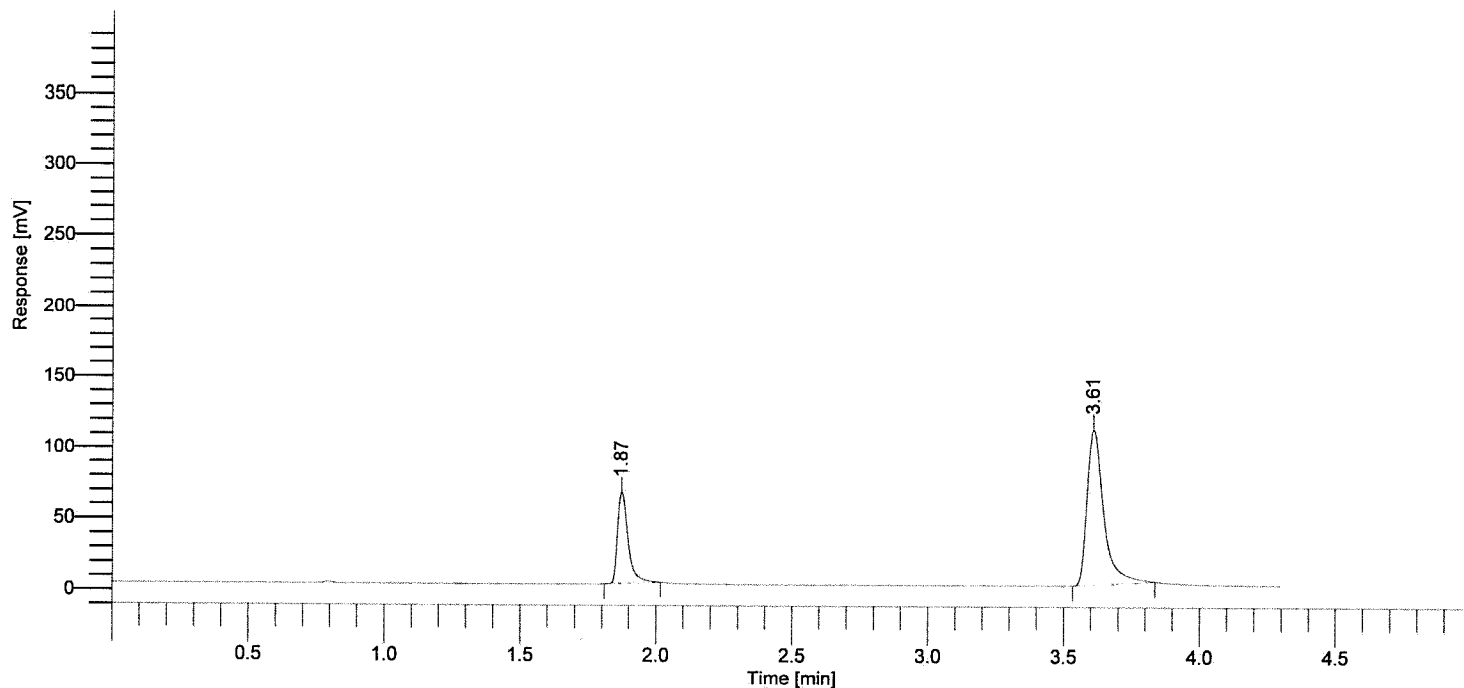

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.61

37

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53485
Sample Name : GUTH 19130 #733
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 18

Date : 6/13/2019 10:45:35 AM
Data Acquisition Time : 6/13/2019 10:41:11 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-018.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

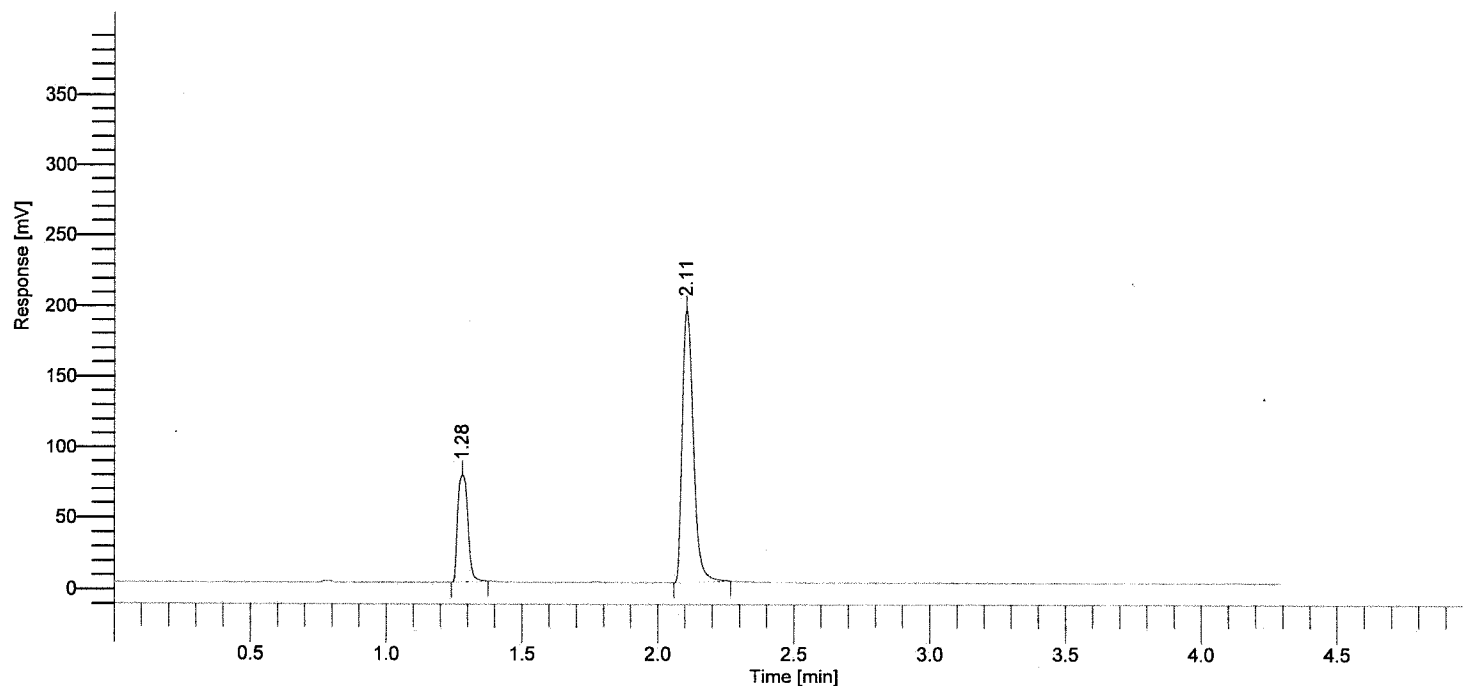

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.1194	1.28	192553.2
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.11	543714.9

38 *CD*

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53486
Sample Name : GUTH 19130 #733
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 18

Date : 6/13/2019 10:45:37 AM
Data Acquisition Time : 6/13/2019 10:41:11 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-018.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

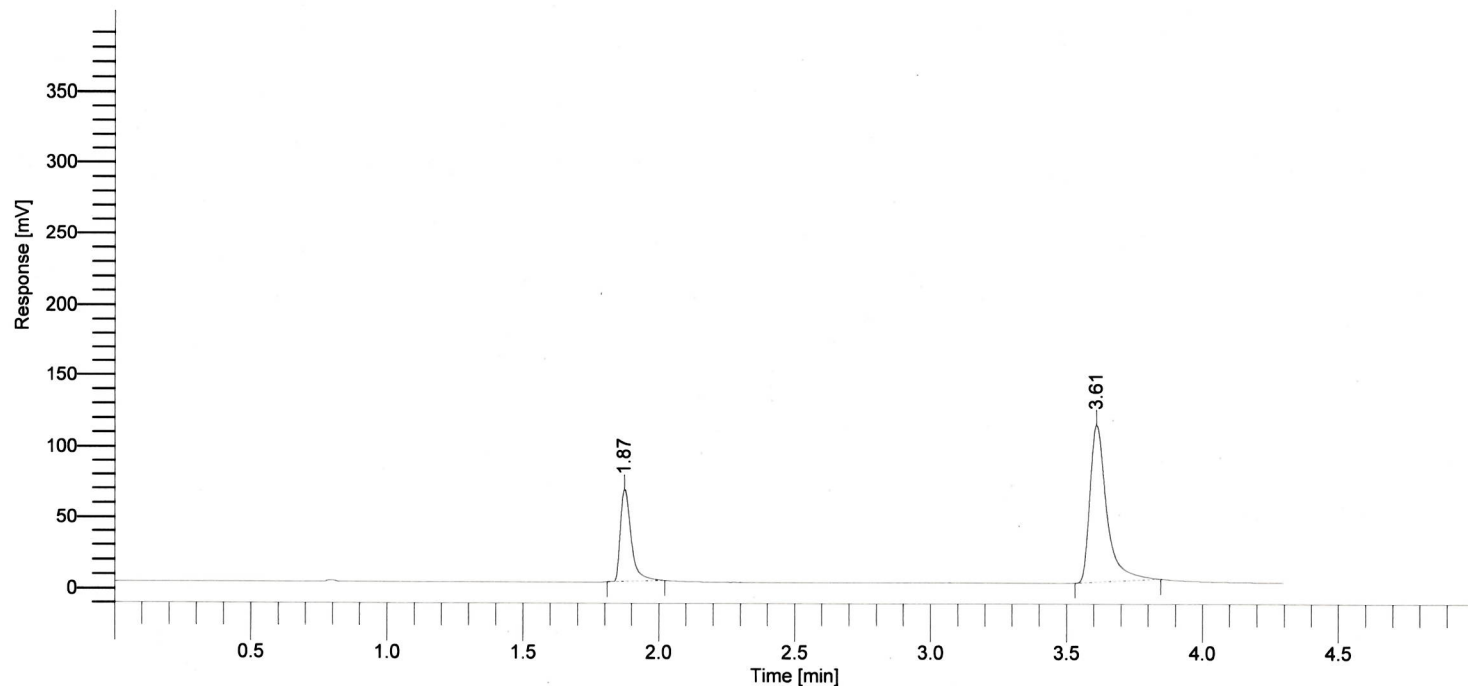

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.61

39 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53487
Sample Name : GUTH 19130 #1445
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 19

Date : 6/13/2019 10:50:35 AM
Data Acquisition Time : 6/13/2019 10:46:11 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-019.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

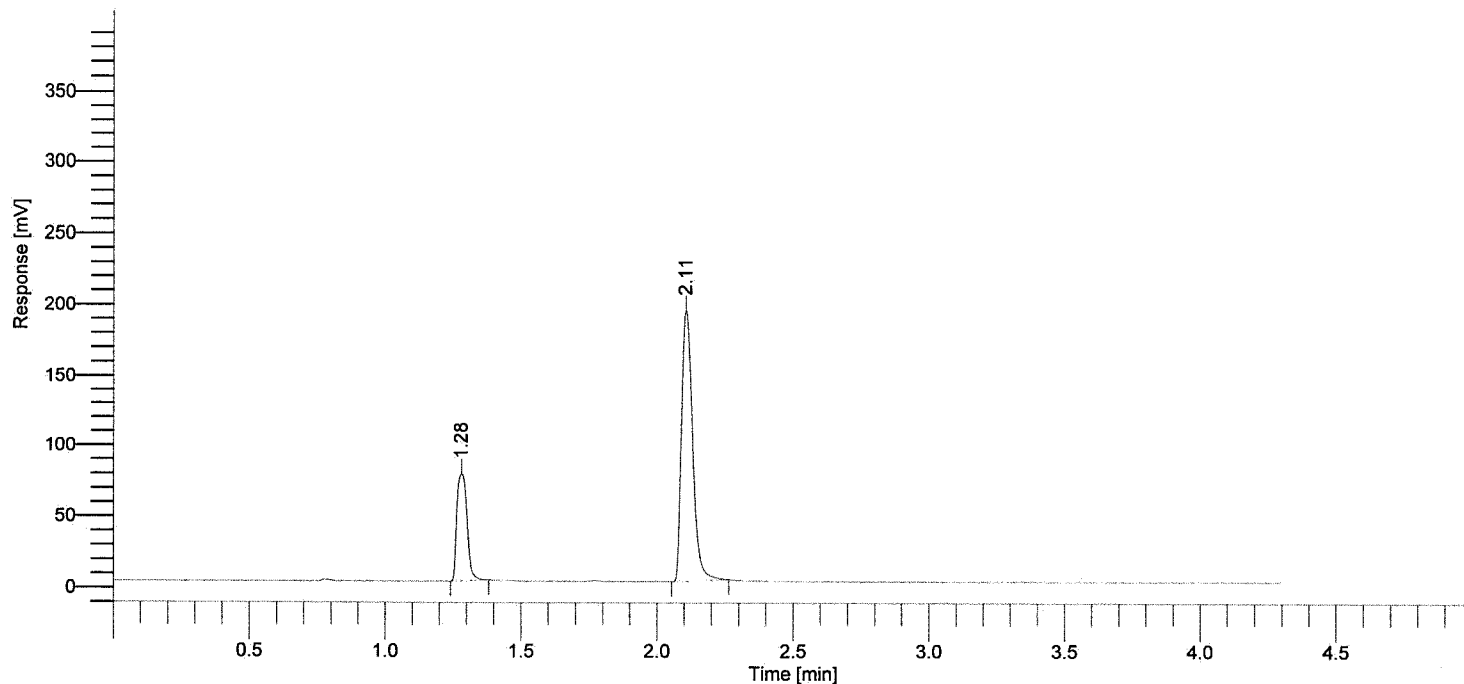

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [μ V·s]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.1193	1.28	192406.6
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.11	543550.8

40 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53488
Sample Name : GUTH 19130 #1445
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 19

Date : 6/13/2019 10:50:37 AM
Data Acquisition Time : 6/13/2019 10:46:11 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-019.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

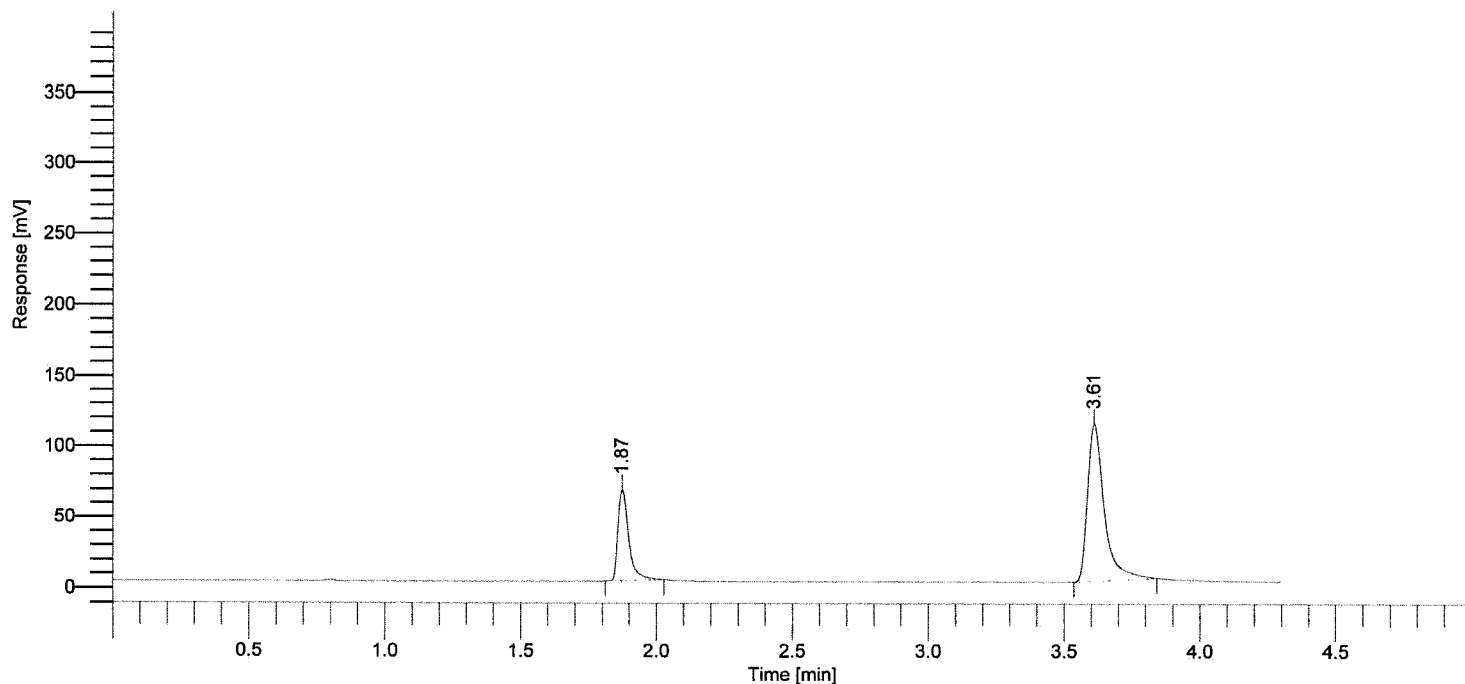

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.61

UIC

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53489
Sample Name : GUTH 19130 #1445
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 20

Date : 6/13/2019 10:55:36 AM
Data Acquisition Time : 6/13/2019 10:51:11 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-020.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

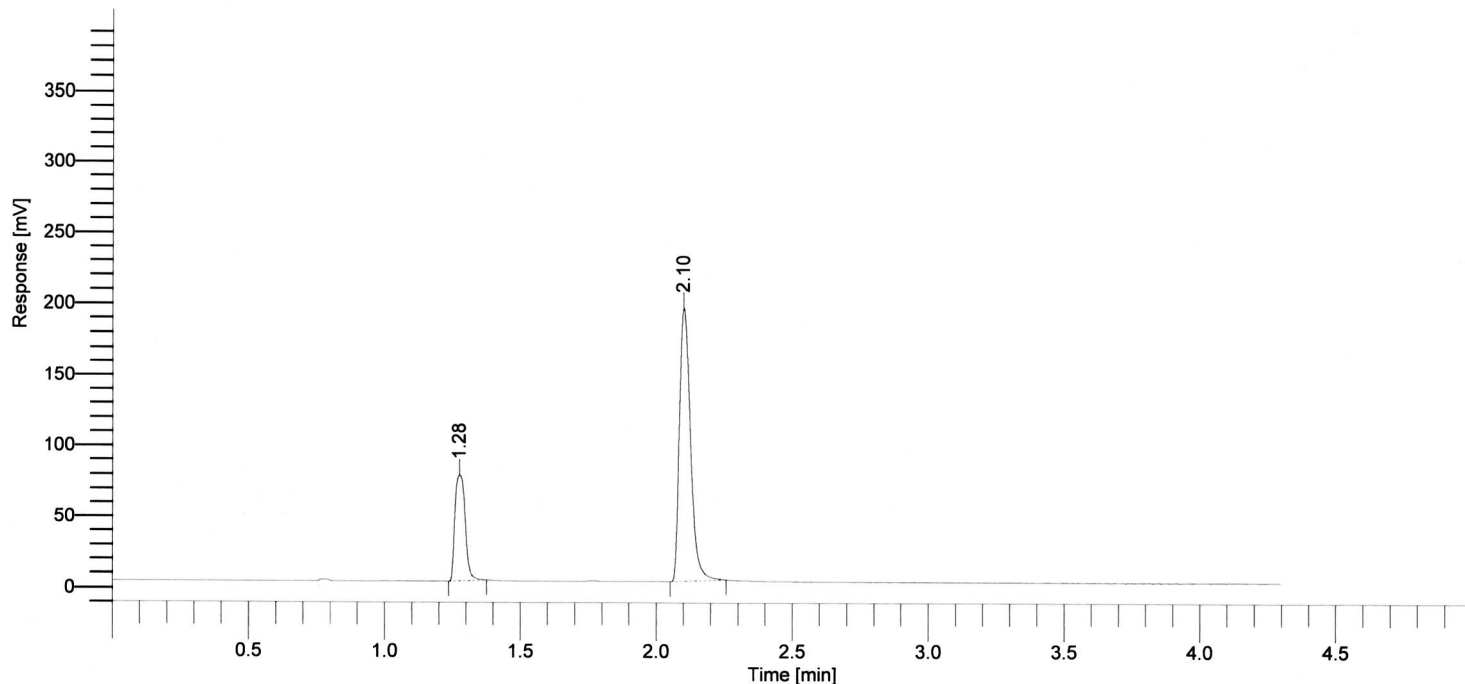

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.1197	1.28	193360.1
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.10	544657.4

42 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53490
Sample Name : GUTH 19130 #1445
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 20

Date : 6/13/2019 10:55:37 AM
Data Acquisition Time : 6/13/2019 10:51:11 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-020.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

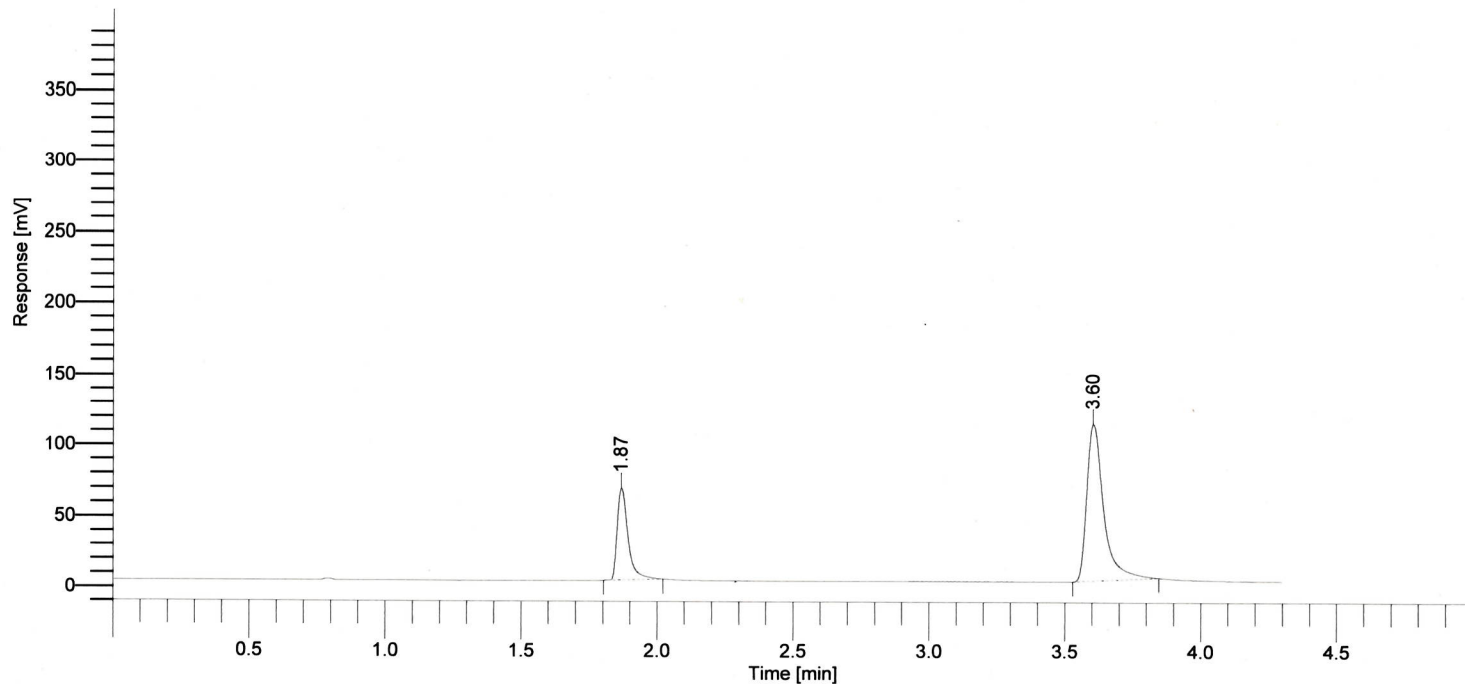

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.60

43 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53491
Sample Name : GUTH 19130 #1445
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 21

Date : 6/13/2019 11:00:36 AM
Data Acquisition Time : 6/13/2019 10:56:11 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-021.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

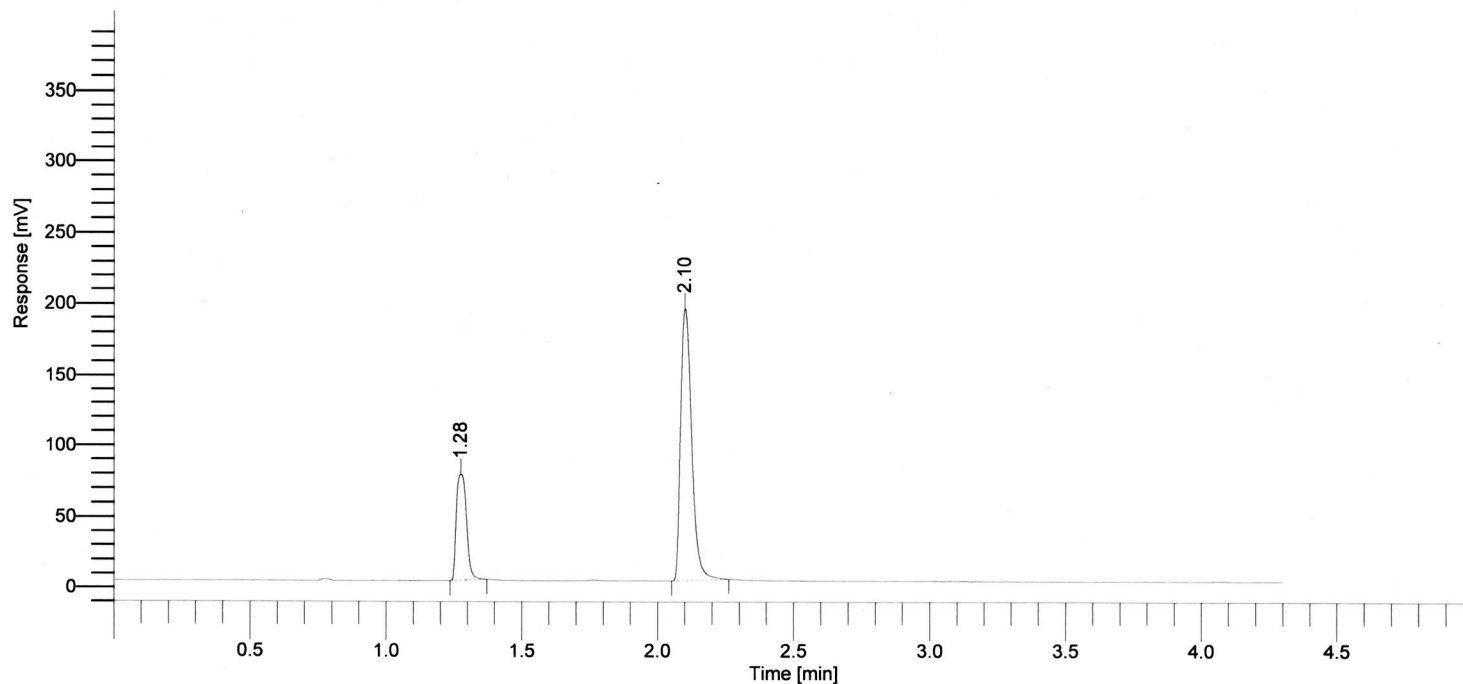

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.1191	1.28	192466.5
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.10	544946.0

44 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53492
Sample Name : GUTH 19130 #1445
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 21

Date : 6/13/2019 11:00:37 AM
Data Acquisition Time : 6/13/2019 10:56:11 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-021.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

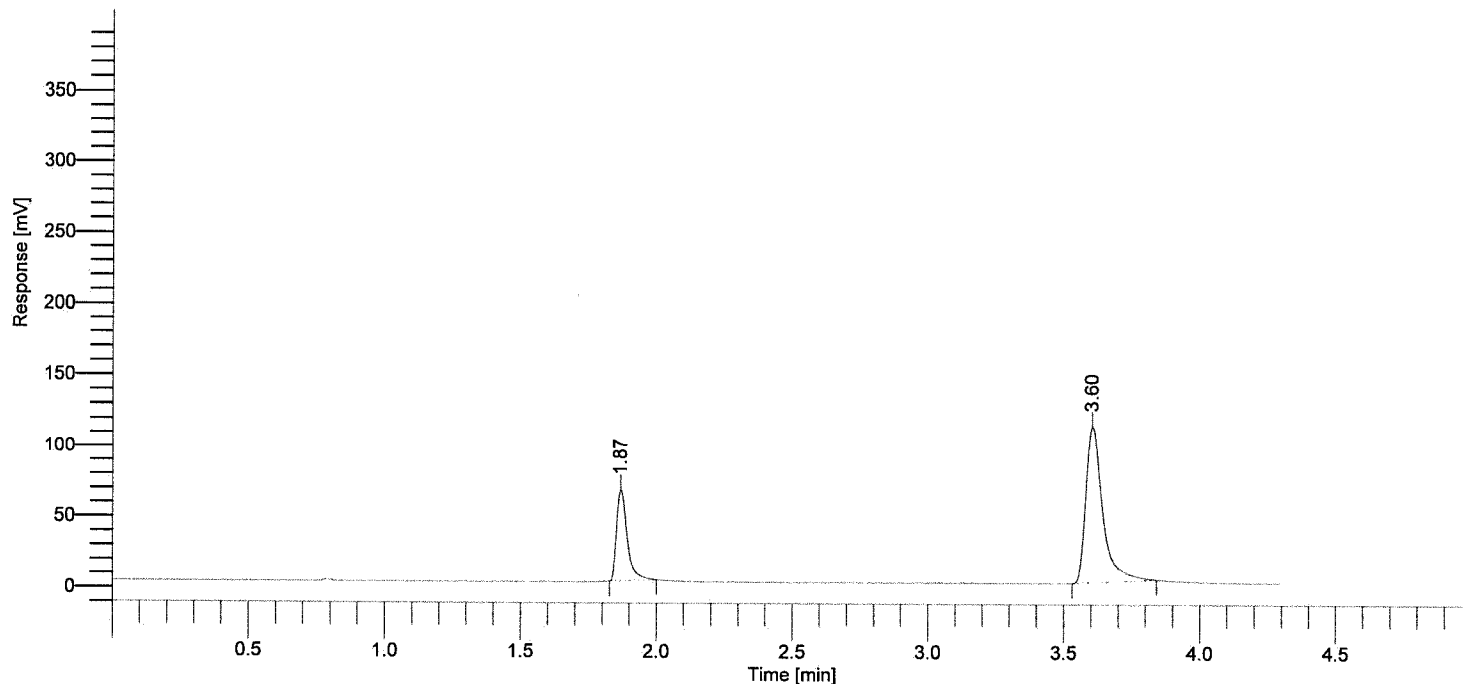

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.60

45 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53493
Sample Name : GUTH 19130 #1446
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 22

Date : 6/13/2019 11:05:33 AM
Data Acquisition Time : 6/13/2019 11:01:08 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-022.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

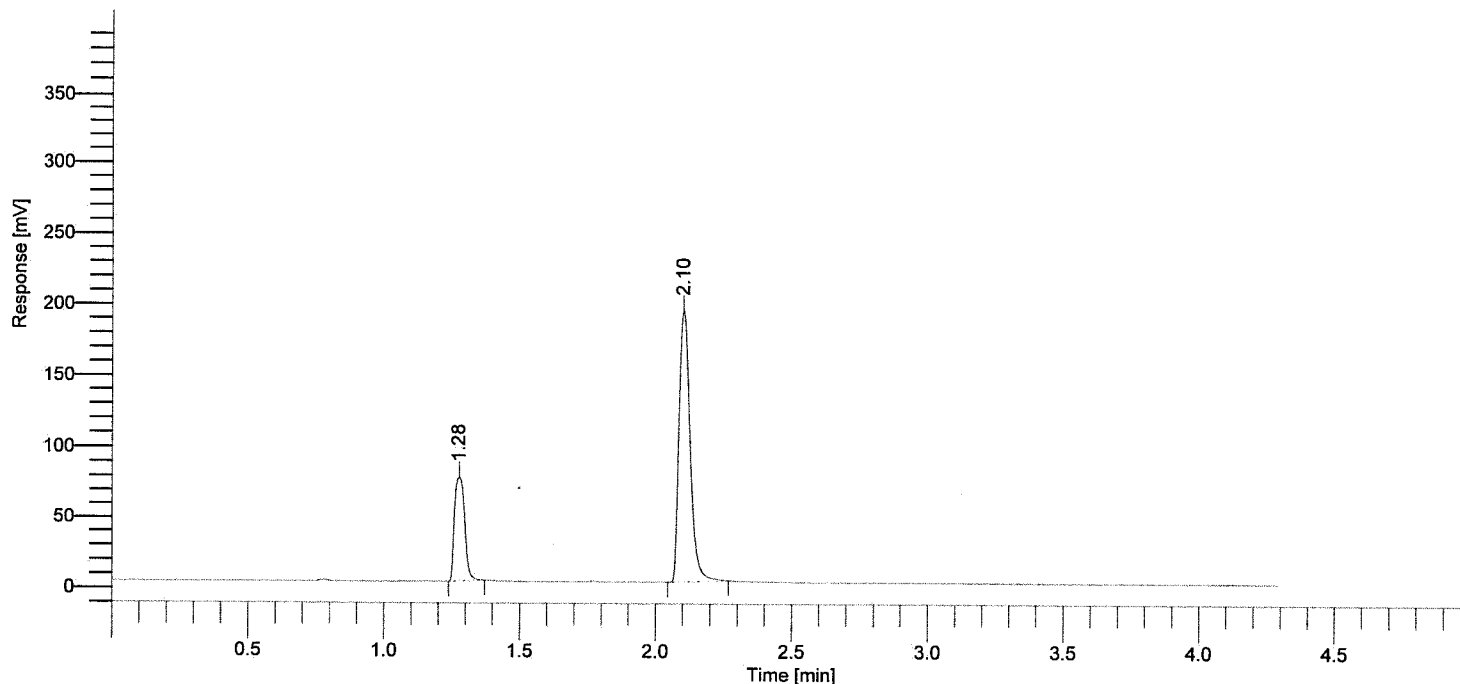

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.1189	1.28	191971.1
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.10	544494.6

4/6 can

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53494
Sample Name : GUTH 19130 #1446
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 22

Date : 6/13/2019 11:05:34 AM
Data Acquisition Time : 6/13/2019 11:01:08 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-022.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

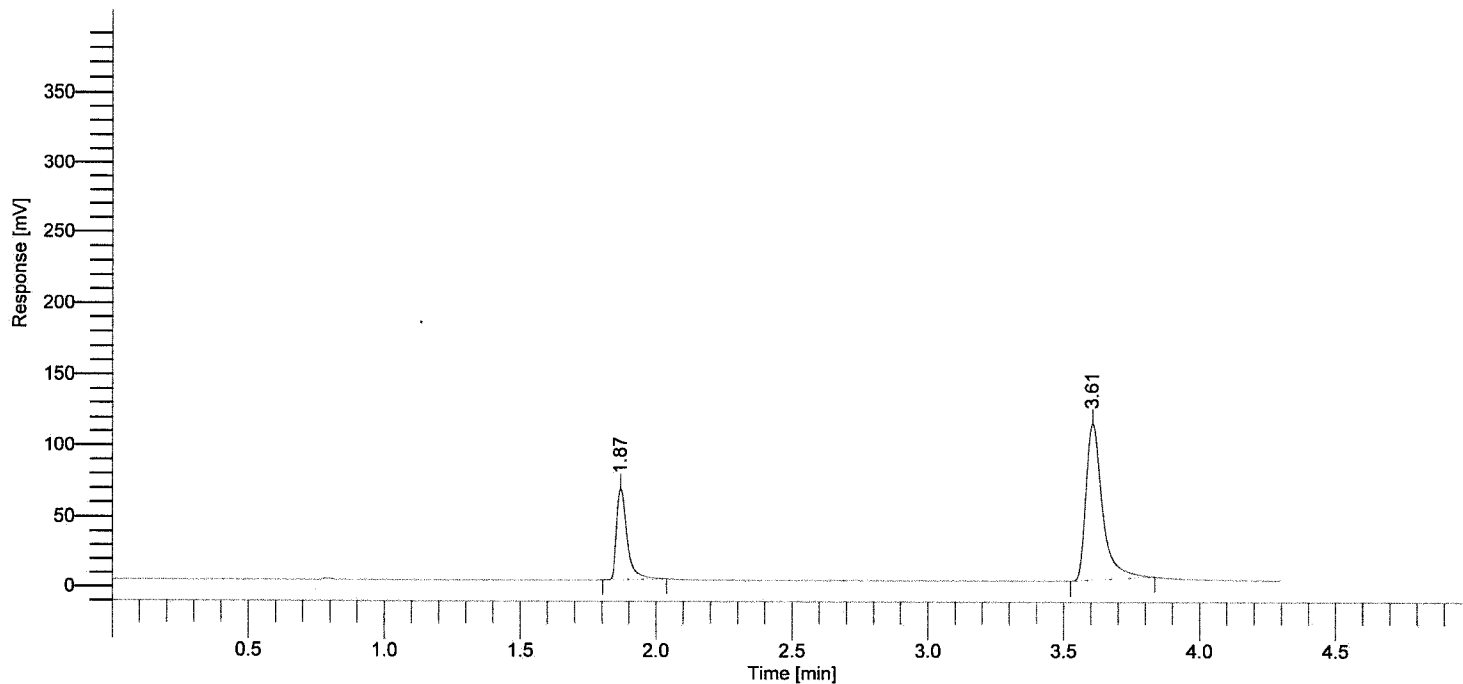

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.61

47

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53495
Sample Name : GUTH 19130 #1446
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 23

Date : 6/13/2019 11:10:33 AM
Data Acquisition Time : 6/13/2019 11:06:08 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-023.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

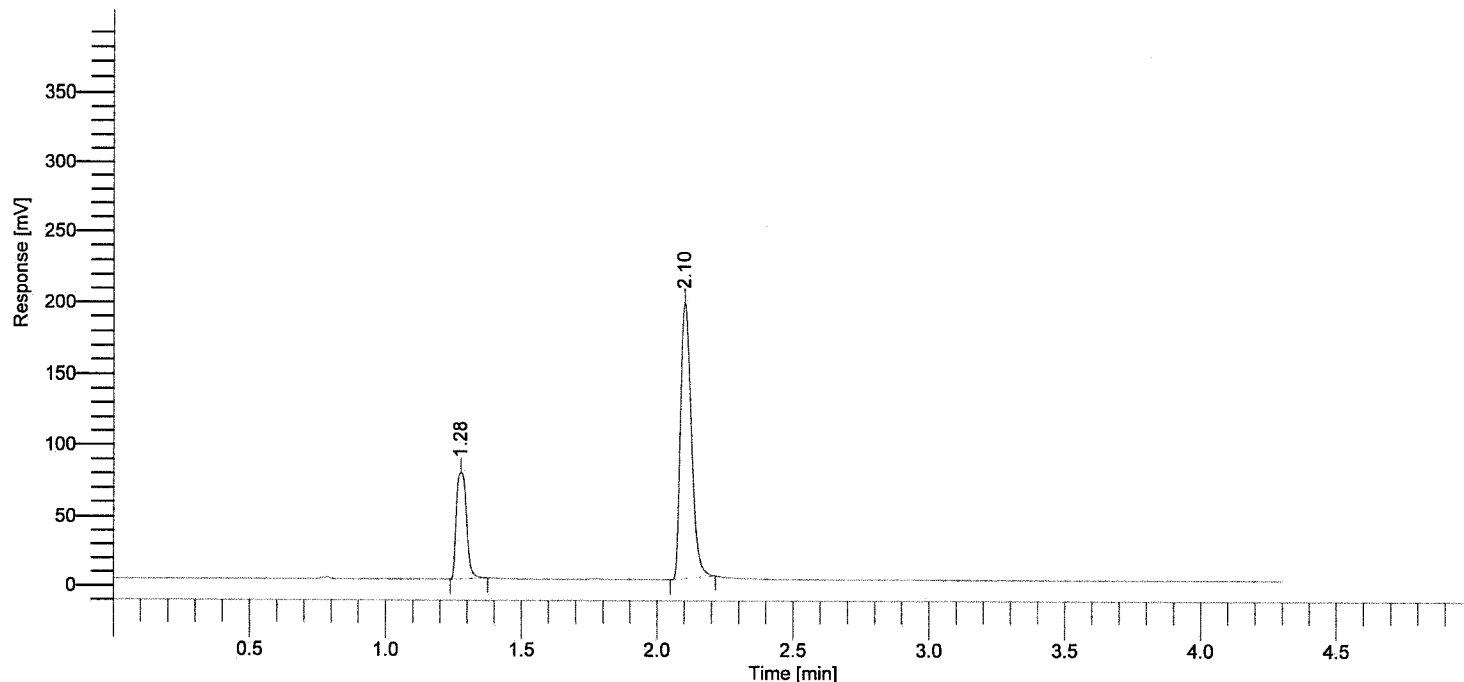

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.1218	1.28	196626.2
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.10	543730.6

48 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53496
Sample Name : GUTH 19130 #1446
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 23

Date : 6/13/2019 11:10:34 AM
Data Acquisition Time : 6/13/2019 11:06:08 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-023.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

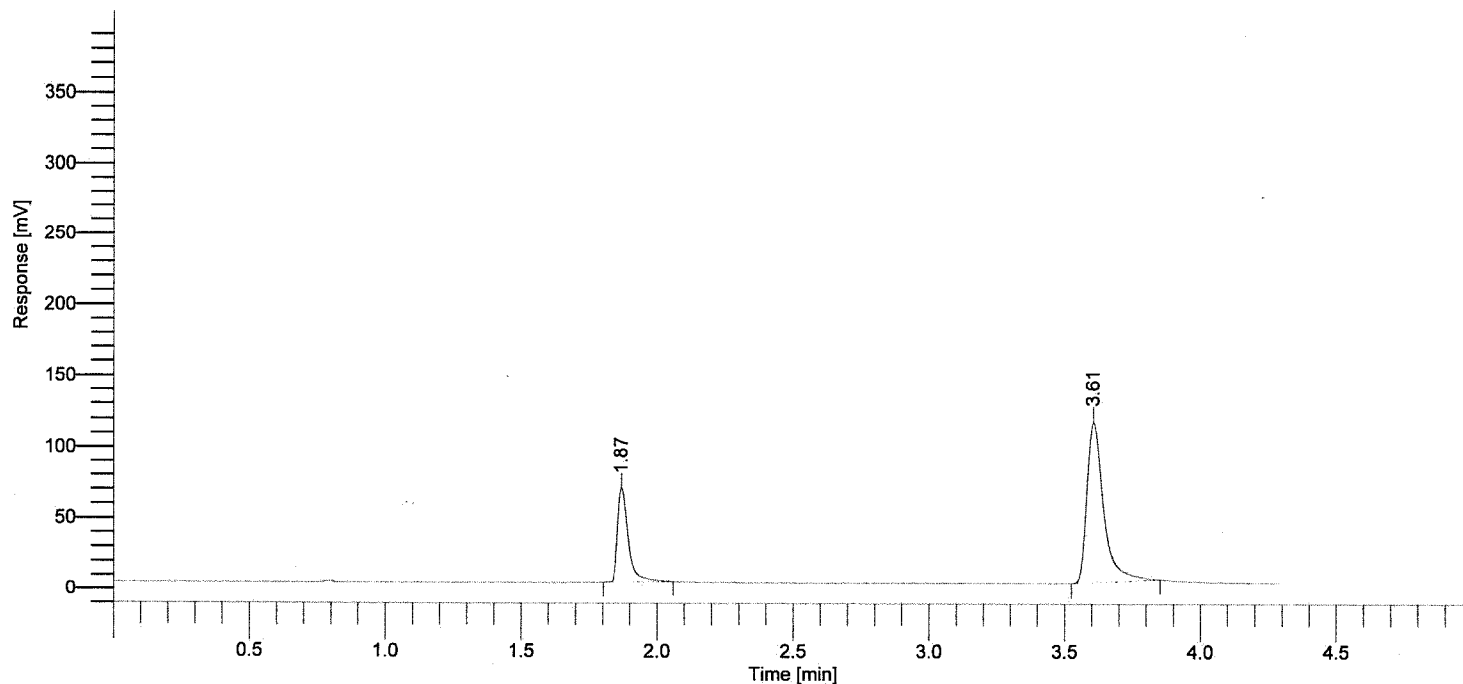

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.61

49 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53497
Sample Name : GUTH 19130 #1446
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 24

Date : 6/13/2019 11:15:33 AM
Data Acquisition Time : 6/13/2019 11:11:08 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-024.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

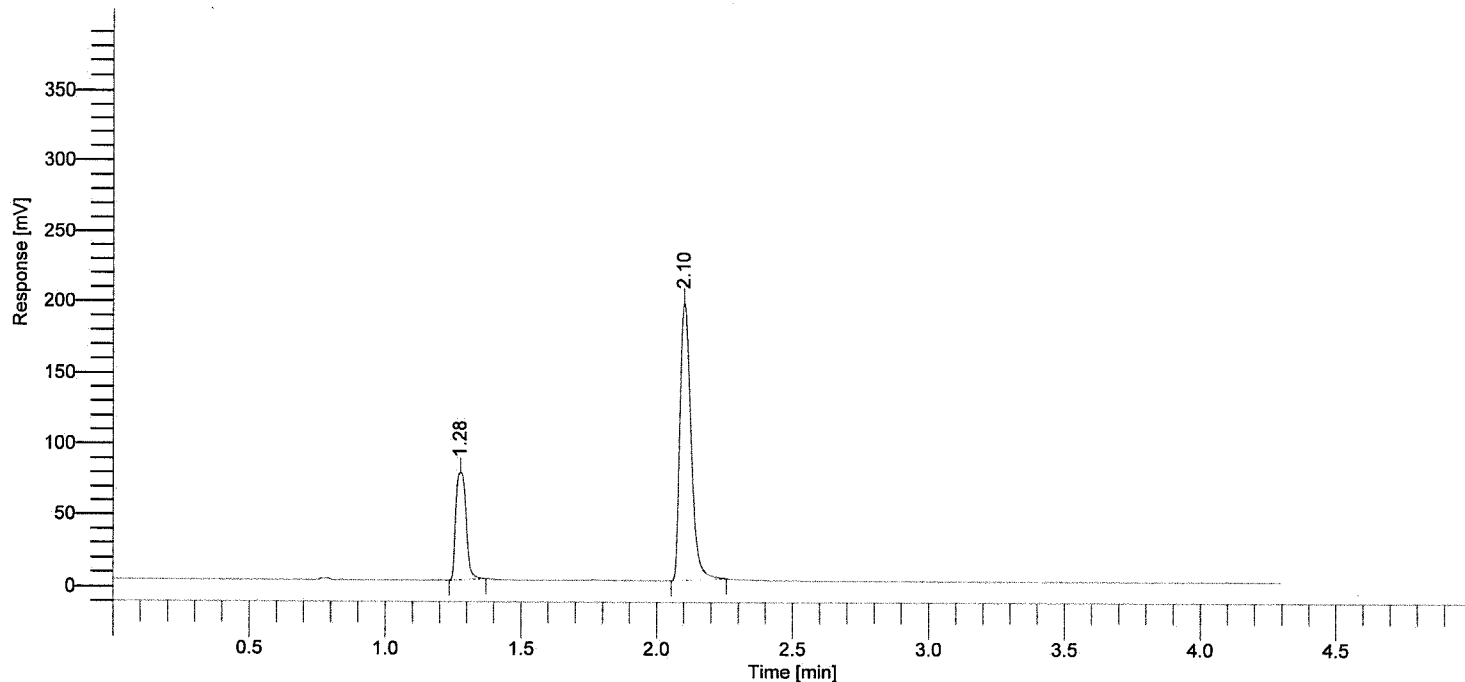

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.1194	1.28	194872.5
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.10	550160.9

50 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53498
Sample Name : GUTH 19130 #1446
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 24

Date : 6/13/2019 11:15:34 AM
Data Acquisition Time : 6/13/2019 11:11:08 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-024.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

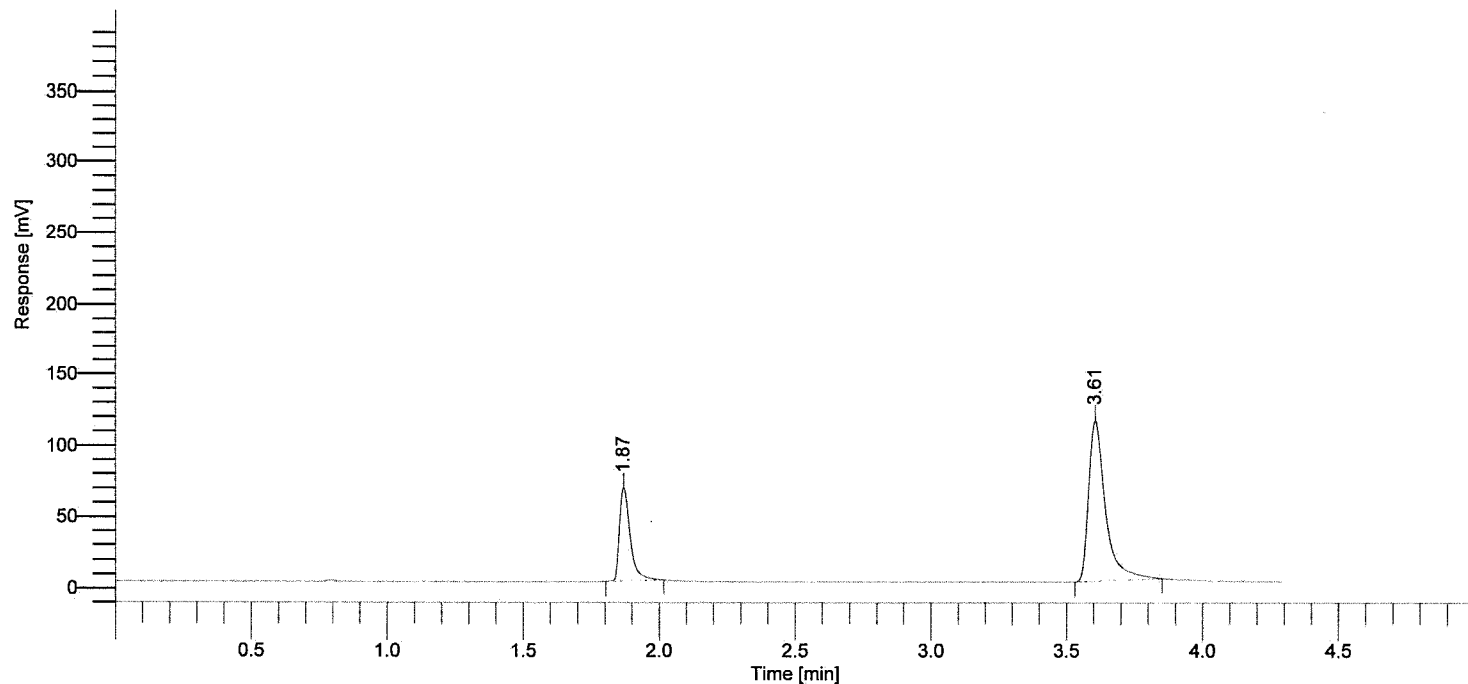

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.61

5162

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53499
Sample Name : 0.10% CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 25

Date : 6/13/2019 11:20:33 AM
Data Acquisition Time : 6/13/2019 11:16:08 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-025.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

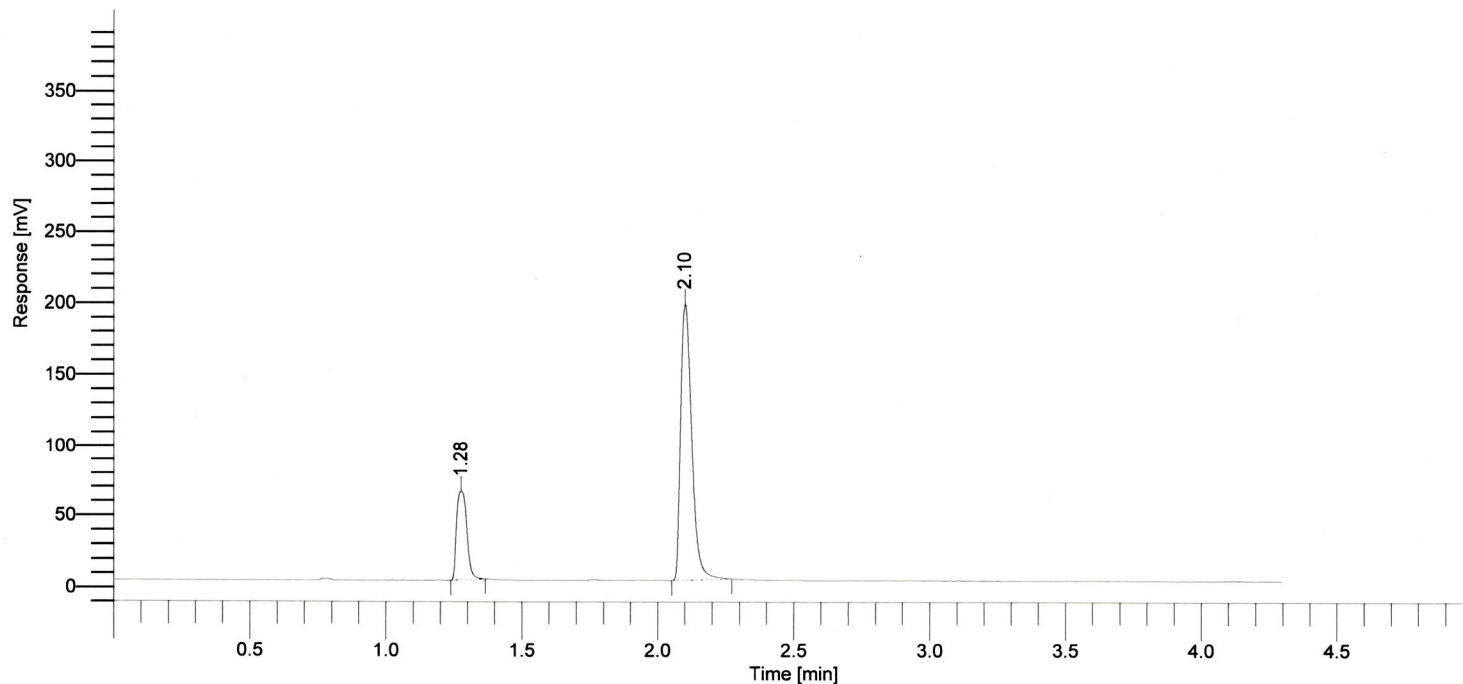

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.0980	1.28	159947.3
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.10	554376.9

52 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53500
Sample Name : 0.10% CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 25

Date : 6/13/2019 11:20:34 AM
Data Acquisition Time : 6/13/2019 11:16:08 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-025.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

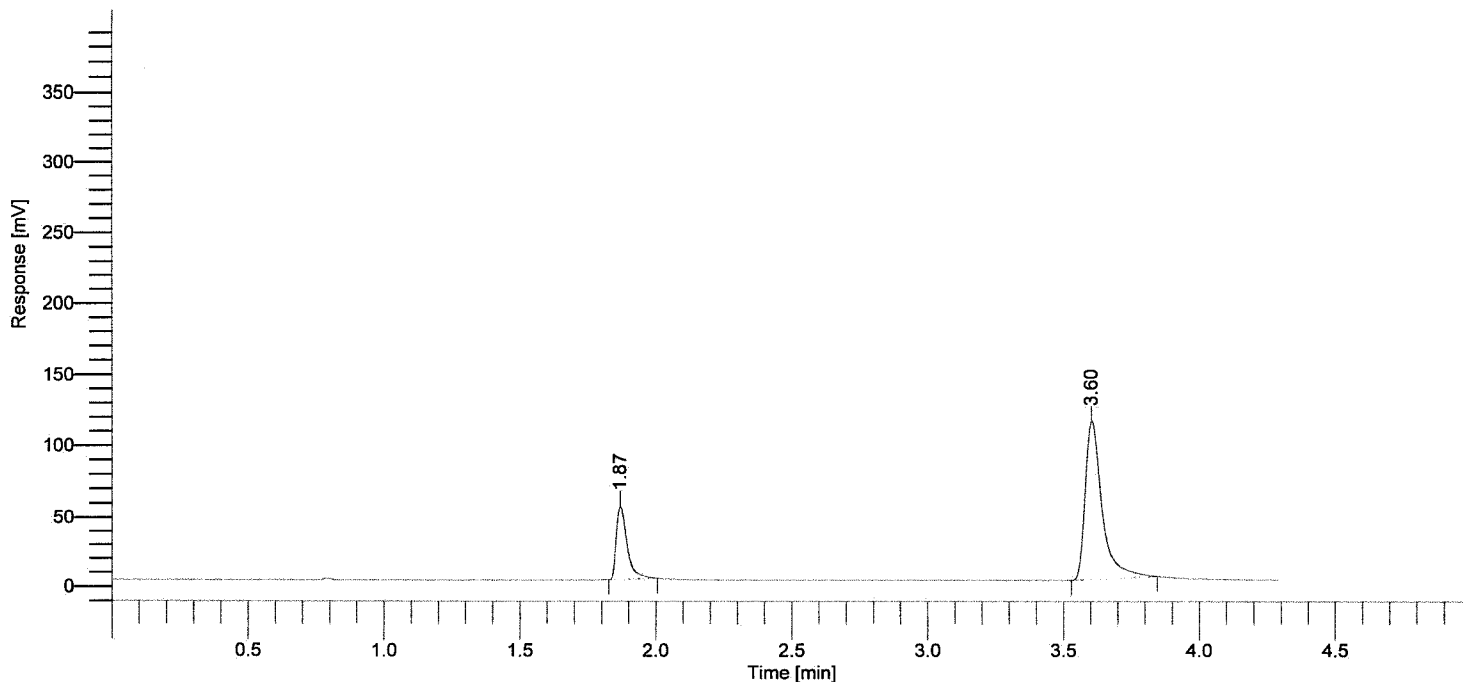

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.60

536

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53501
Sample Name : 0.20% CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 26

Date : 6/13/2019 11:25:33 AM
Data Acquisition Time : 6/13/2019 11:21:08 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-026.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

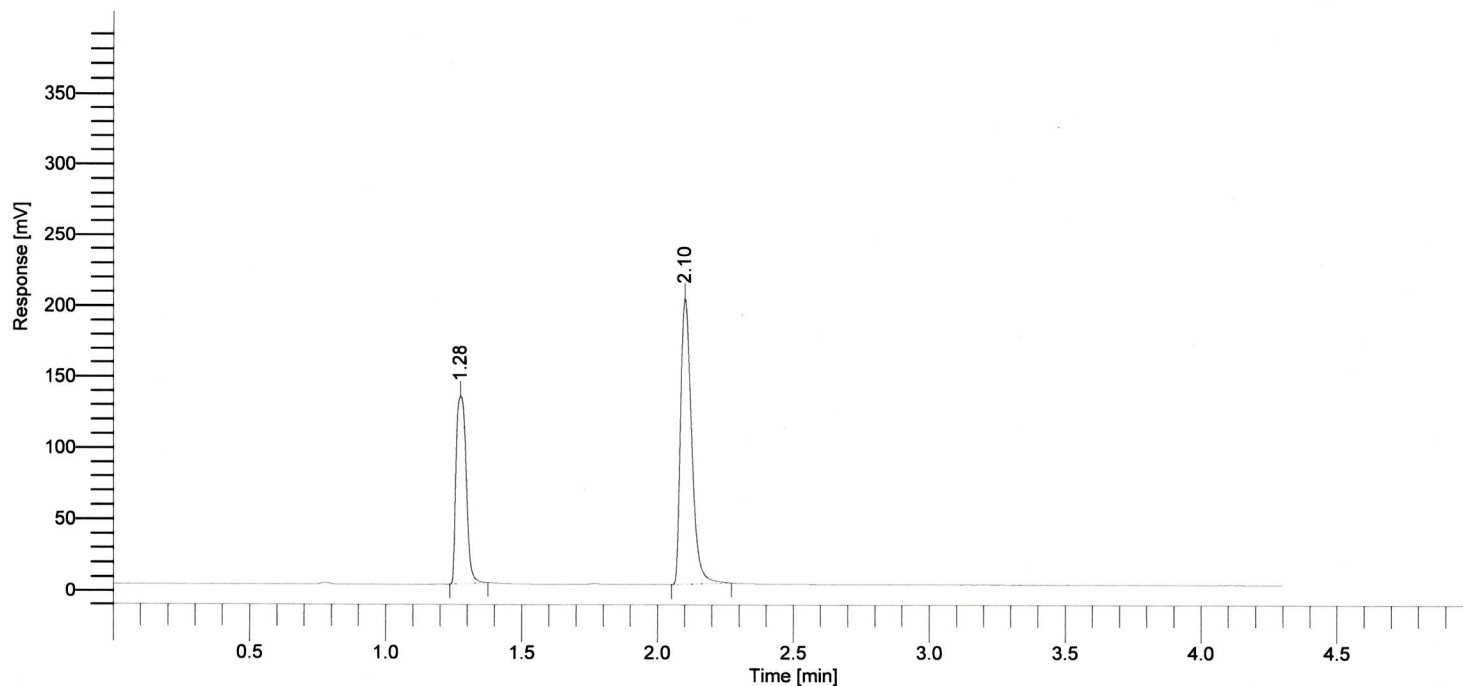

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.1967	1.28	335137.1
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.10	567091.2

54 cm

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53502
Sample Name : 0.20% CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 26

Date : 6/13/2019 11:25:34 AM
Data Acquisition Time : 6/13/2019 11:21:08 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-026.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

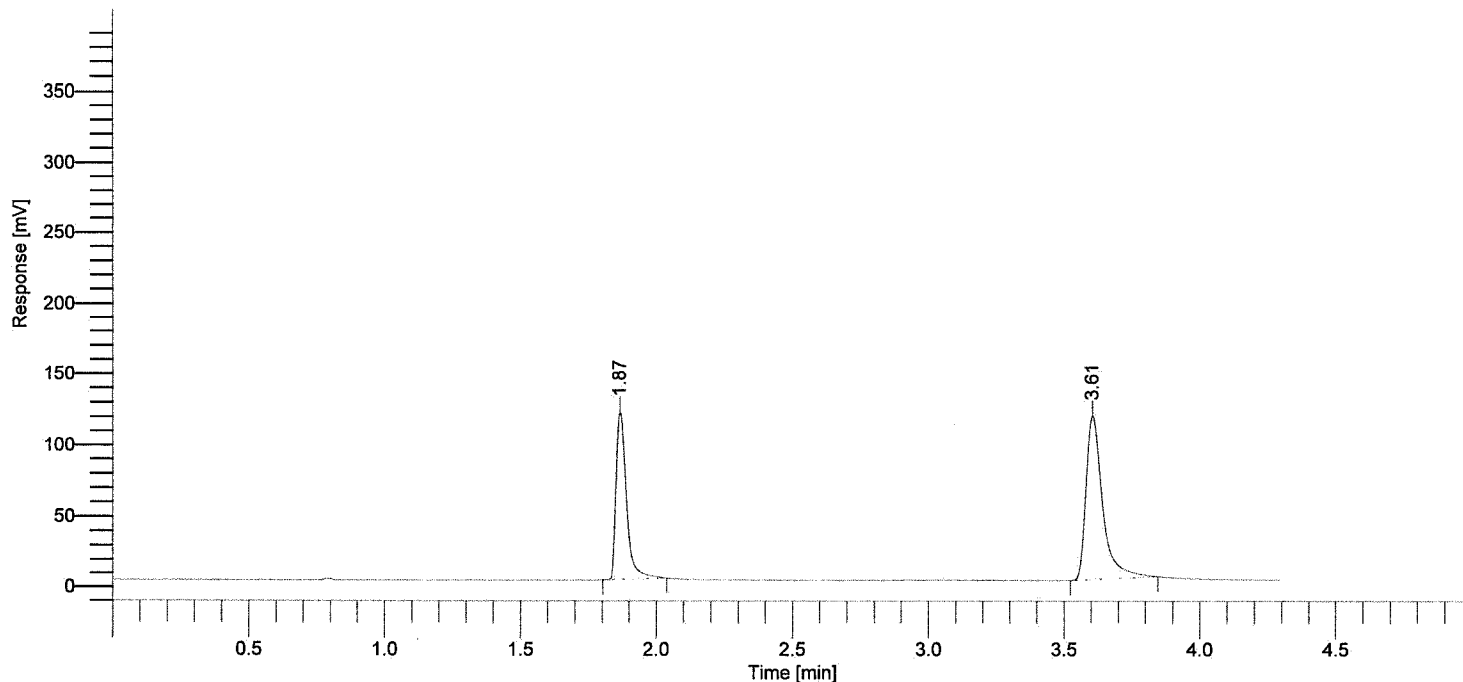

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"


Component Name	Time [min]
ETHANOL	1.87
N-PROPANOL	3.61

SS *cm*

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53503
Sample Name : NEG CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 27

Date : 6/13/2019 11:30:33 AM
Data Acquisition Time : 6/13/2019 11:26:08 AM
Channel : A
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\A20190613-027.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

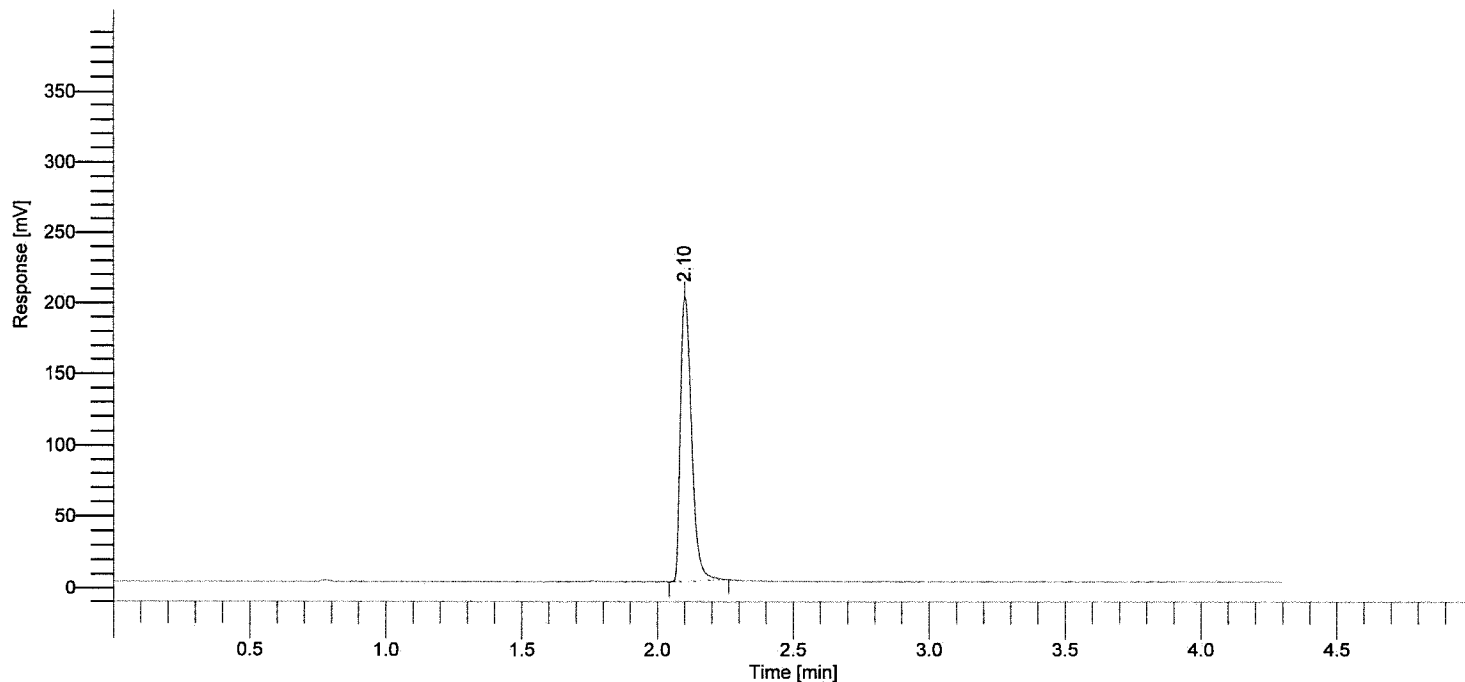

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC1 COLUMN ON FID "A"


Component Name	% by Wt	Time [min]	Area [$\mu\text{V}\cdot\text{s}$]
METHANOL	0.0000	1.02	0.0
ETHANOL	0.0000	1.28	0.0
ISOPROPANOL	0.0000	1.56	0.0
ACETONE	0.0000	1.93	0.0
N-PROPANOL	-----	2.10	569092.6

56 Gen

Software Version : 6.3.2.0646
Reprocess Number : d-2ua3120y7b: 53504
Sample Name : NEG CONTROL
Instrument Name : GCHeadspace2
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 27

Date : 6/13/2019 11:30:34 AM
Data Acquisition Time : 6/13/2019 11:26:08 AM
Channel : B
Operator : manager
Dilution Factor : 1.000000

Result File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Data\B20190613-027.rst
Sequence File : C:\PenExe1\TcWS\Ver6.3.2\GCHeadspace2\Sequences\SimSoln.seq

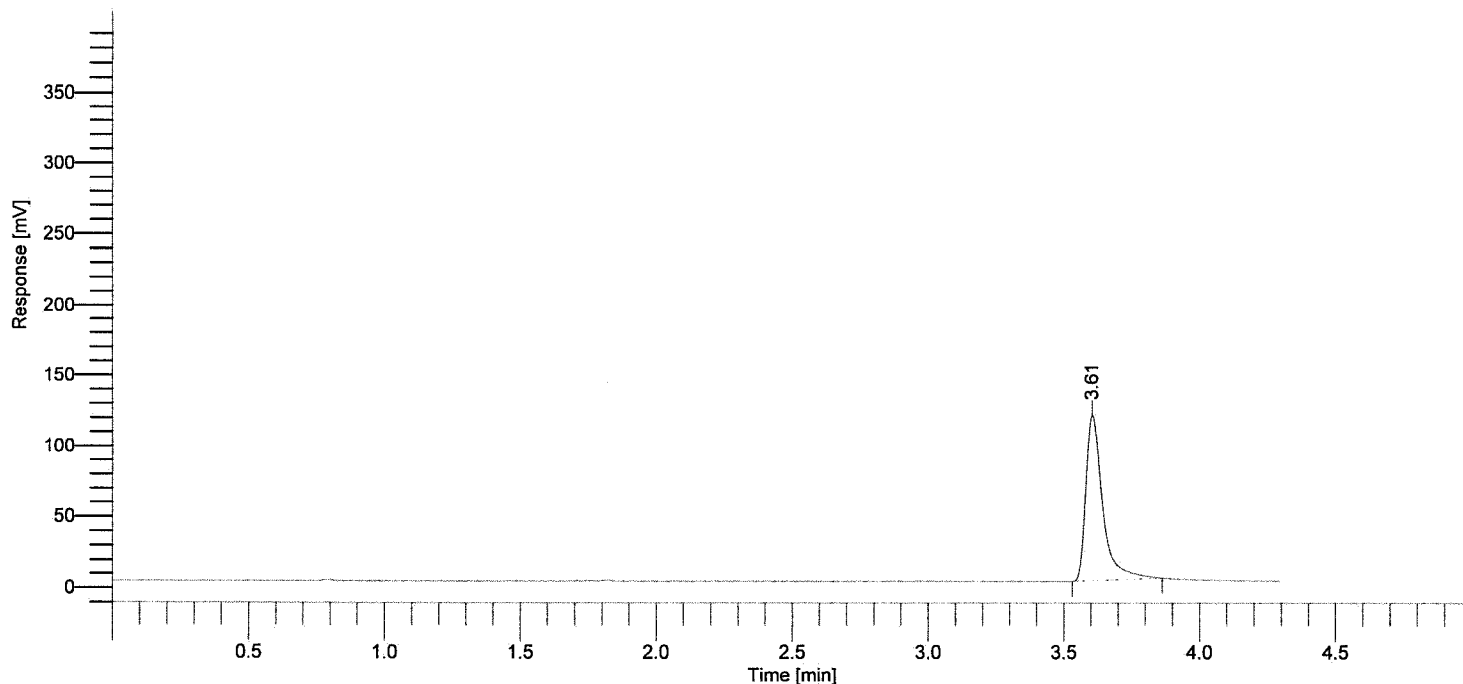

BLOOD ALCOHOL REPORT NYSP

RESULTS FROM BAC2 COLUMN ON FID "B"

Component Name	Time [min]
N-PROPANOL	3.61

57 cm